

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AS

Instrument ID : Konelab

3/13/2019 12:43

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.882	0.0	0.092	
ICB1	0.485	0.0	0.004	
CCV1	243.233	0.0	0.225	
CCB1	0.165	0.0	0.004	
PB117855BL	0.424	0.0	0.004	
PB117855BS	97.805	0.0	0.093	
K1847-14	1.123	0.0	0.005	
K1847-14DUP	1.228	0.0	0.005	
K1847-14MS	33.314	0.0	0.034	
K1847-14MSD	33.437	0.0	0.034	
K1847-15	0.992	0.0	0.005	
K1847-16	1.667	0.0	0.006	
K1847-17	1.915	0.0	0.006	
K1847-18	2.320	0.0	0.006	
CCV2	246.046	0.0	0.227	
CCB2	0.570	0.0	0.005	
PB117856BL	0.492	0.0	0.004	
PB117856BS	99.053	0.0	0.094	
K1844-02	2.548	0.0	0.006	
K1844-02DUP	2.505	0.0	0.006	
K1844-02MS	34.132	0.0	0.035	
K1844-02MSD	33.453	0.0	0.034	
HIGHPB117855	509.327	0.0	0.466	Test limit high
K1833-24	922.858	0.0	0.841	Test limit high
CCV3	252.351	0.0	0.233	
CCB3	0.177	0.0	0.004	
LOWPB117855	10.052	0.0	0.013	
K1833-24DLX5	290.460	0.0	0.268	
CCV4	254.452	0.0	0.235	
CCB4	0.077	0.0	0.004	

N 30
Mean 105.785
SD 198.3787
CV% 187.53

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

3/13/2019 10:11


Test Total CN

Accepted 3/13/2019 10:11

Factor 1102
Bias 0.004

Coeff. of det. 0.999998

Errors

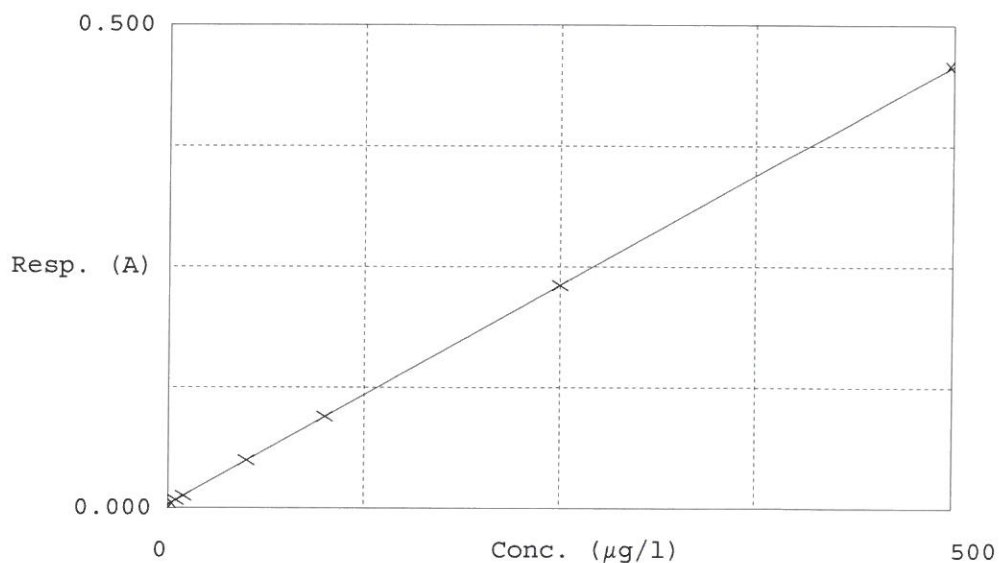

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.3651	0.0000	
2	5.0PPBCN	0.008	4.7637	5.0000	
3	10PPBCN	0.013	9.6897	10.0000	
4	50PPBCN	0.050	50.2264	50.0000	
5	100PPBCN	0.095	100.1116	100.0000	
6	250PPBCN	0.231	249.7596	250.0000	
7	500PPBCN	0.458	500.0838	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Wed Mar 13 10:11:09 2019

Wed Mar 13 12:41:00 2019

AS

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.3651	µg/l	3/13/2019 10:11:09	
5.0PPBCN	A	Total CN	P	4.7637	µg/l	3/13/2019 10:11:10	
10PPBCN	A	Total CN	P	9.6897	µg/l	3/13/2019 10:11:11	
50PPBCN	A	Total CN	P	50.2264	µg/l	3/13/2019 10:11:12	
100PPBCN	A	Total CN	P	100.1116	µg/l	3/13/2019 10:11:13	
250PPBCN	A	Total CN	P	249.7596	µg/l	3/13/2019 10:11:14	
500PPBCN	A	Total CN	P	500.0838	µg/l	3/13/2019 10:11:15	
ICV1	S	Total CN	P	96.8825	µg/l	3/13/2019 11:00:26	
ICB1	S	Total CN	P	0.4848	µg/l	3/13/2019 11:00:27	
CCV1	S	Total CN	P	243.2334	µg/l	3/13/2019 11:00:28	
CCB1	S	Total CN	P	0.165	µg/l	3/13/2019 11:00:29	
PB117855BL	S	Total CN	P	0.4239	µg/l	3/13/2019 11:00:30	
PB117855BS	S	Total CN	P	97.8053	µg/l	3/13/2019 11:00:31	
K1847-14	S	Total CN	P	1.1229	µg/l	3/13/2019 11:00:32	
K1847-14DUP	S	Total CN	P	1.2282	µg/l	3/13/2019 11:00:33	
K1847-14MS	S	Total CN	P	33.3143	µg/l	3/13/2019 11:00:34	
K1847-14MSD	S	Total CN	P	33.4375	µg/l	3/13/2019 11:00:35	
K1847-15	S	Total CN	P	0.9921	µg/l	3/13/2019 11:00:36	
K1847-16	S	Total CN	P	1.6669	µg/l	3/13/2019 11:07:59	
K1847-17	S	Total CN	P	1.9148	µg/l	3/13/2019 11:08:00	
K1847-18	S	Total CN	P	2.3197	µg/l	3/13/2019 11:08:01	
CCV2	S	Total CN	P	246.0455	µg/l	3/13/2019 11:08:02	
CCB2	S	Total CN	P	0.5695	µg/l	3/13/2019 11:08:03	
PB117856BL	S	Total CN	P	0.4917	µg/l	3/13/2019 11:08:04	
PB117856BS	S	Total CN	P	99.0529	µg/l	3/13/2019 11:08:05	
K1844-02	S	Total CN	P	2.5482	µg/l	3/13/2019 11:08:06	
K1844-02DUP	S	Total CN	P	2.5054	µg/l	3/13/2019 11:08:07	
K1844-02MS	S	Total CN	P	34.1324	µg/l	3/13/2019 11:08:08	
K1844-02MSD	S	Total CN	P	33.4528	µg/l	3/13/2019 11:08:09	
HIGHPB117855	S	Total CN	P	509.3265	µg/l	3/13/2019 11:13:43	
K1833-24	S	Total CN	P	922.8583	µg/l	3/13/2019 11:13:46	
CCV3	S	Total CN	P	252.3513	µg/l	3/13/2019 11:13:47	
CCB3	S	Total CN	P	0.1774	µg/l	3/13/2019 11:13:48	
LOWPB117855	S	Total CN	P	10.0521	µg/l	3/13/2019 11:42:31	
K1833-24DLX5	S	Total CN	P	290.4601	µg/l	3/13/2019 11:42:33	
CCV4	S	Total CN	P	254.4523	µg/l	3/13/2019 11:59:05	
CCB4	S	Total CN	P	0.0773	µg/l	3/13/2019 11:59:06	