


LB101339

7470A

INSTRUMENT ID : CV1

 μ Abs. :

44980

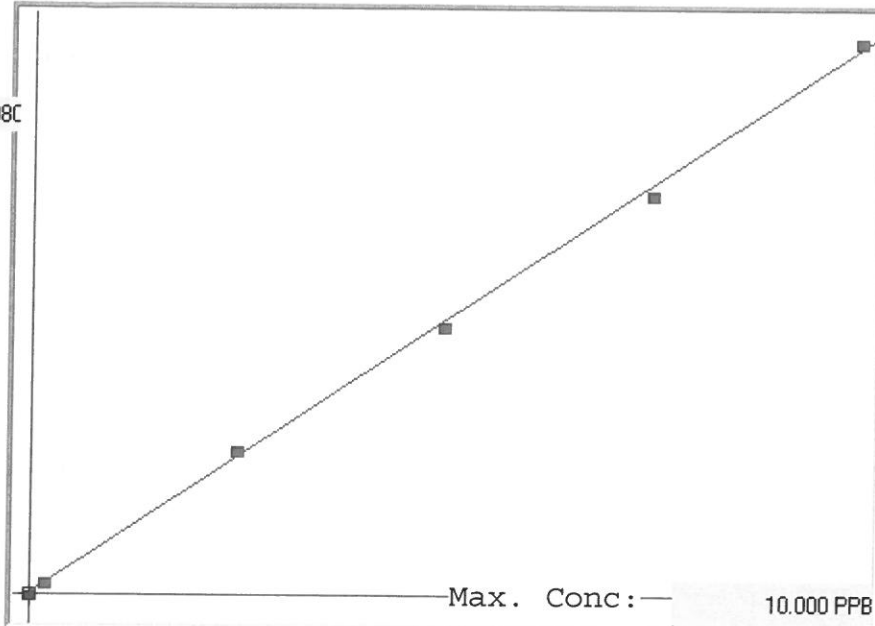

Linear

A= 0.0000e+000

B= 2.2541e-004

C= -1.8220e-002

Rho= 0.9996132

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.012	-0.012	27	0.000	27				
0.2	0.200	0.204	0.004	985	0.0 %	985				
2.5	2.500	2.631	0.131	11751	0.0 %	11751				
5.0	5.000	4.910	-0.090	21864	0.0 %	21864				
7.5	7.500	7.347	-0.153	32676	0.0 %	32676				
10.0	10.000	10.121	0.121	44980	0.0 %	44980				

LB101339 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 13 Mar 2019 14:12:27

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	27	-	0.0000	7470A	PPB	13 Mar 2019 14:14:59	S	Std
0.2 - 1	50-2	985	-	0.2000	7470A	PPB	13 Mar 2019 14:17:07	S	Std
2.5 - 1	52-5	11751	-	2.5000	7470A	PPB	13 Mar 2019 14:19:15	S	Std
5.0 - 1	55-0	21864	-	5.0000	7470A	PPB	13 Mar 2019 14:21:23	S	Std
7.5 - 1	57-5	32676	-	7.5000	7470A	PPB	13 Mar 2019 14:23:31	S	Std
10.0 - 1	510-0	44980	-	10.0000	7470A	PPB	13 Mar 2019 14:30:40	S	Std
ICV53 - 1	ICV53	16937	3.7995	-	7470A	PPB	13 Mar 2019 14:35:37	U	SMPL
ICB53 - 1	ICB53	-27	-0.0243	-	7470A	PPB	13 Mar 2019 14:37:43	U	SMPL
CCV54 - 1	CCV54	21943	4.9279	-	7470A	PPB	13 Mar 2019 14:39:49	U	SMPL
CCB54 - 1	CCB54	-21	-0.0230	-	7470A	PPB	13 Mar 2019 14:41:54	U	SMPL
CRA - 1	CRA	919	0.1889	-	7470A	PPB	13 Mar 2019 14:44:00	U	SMPL
HighStd - 1	HighStd	42607	9.5857	-	7470A	PPB	13 Mar 2019 14:46:07	U	SMPL
ChkStd - 1	ChkStd	31104	6.9928	-	7470A	PPB	13 Mar 2019 14:48:13	U	SMPL
PB117877BL - 1	PBW	43	-0.0085	-	7470A	PPB	13 Mar 2019 14:50:21	U	SMPL
PB117877BS - 1	LCSW	18984	4.2609	-	7470A	PPB	13 Mar 2019 14:52:28	U	SMPL
K1687-02 - 1	HR-06-031119-A	75	-0.0013	-	7470A	PPB	13 Mar 2019 14:54:35	U	SMPL
K1687-02DUP - 1	HR-06-031119-ADUP	113	0.0073	-	7470A	PPB	13 Mar 2019 14:56:43	U	SMPL
K1687-02MS - 1	HR-06-031119-AMS	18089	4.0592	-	7470A	PPB	13 Mar 2019 14:58:51	U	SMPL
K1687-02MSD - 1	HR-06-031119-AMSD	17716	3.9751	-	7470A	PPB	13 Mar 2019 15:00:59	U	SMPL
K1687-04 - 1	HR-06-031119-B	12	-0.0155	-	7470A	PPB	13 Mar 2019 15:03:05	U	SMPL
CCV55 - 1	CCV55	21755	4.8855	-	7470A	PPB	13 Mar 2019 15:05:11	U	SMPL
CCB55 - 1	CCB55	-31	-0.0252	-	7470A	PPB	13 Mar 2019 15:07:18	U	SMPL
K1687-06 - 1	HR-06-031119-C	80	-0.0002	-	7470A	PPB	13 Mar 2019 15:09:24	U	SMPL
K1697-02 - 1	SU-03-031119-A	63	-0.0040	-	7470A	PPB	13 Mar 2019 15:11:30	U	SMPL
K1697-04 - 1	SU-03-031119-B	67	-0.0031	-	7470A	PPB	13 Mar 2019 15:13:36	U	SMPL
K1697-06 - 1	SU-04-031119-A	284	0.0458	-	7470A	PPB	13 Mar 2019 15:15:43	U	SMPL
K1697-08 - 1	SU-04-031119-B	99	0.0041	-	7470A	PPB	13 Mar 2019 15:17:50	U	SMPL
K1844-10 - 1	TOTE-1-3	127	0.0104	-	7470A	PPB	13 Mar 2019 15:19:57	U	SMPL
K1845-01 - 1	ETGI-294	82	0.0003	-	7470A	PPB	13 Mar 2019 15:22:04	U	SMPL
K1846-04 - 1	TP-2	81	0.0000	-	7470A	PPB	13 Mar 2019 15:24:12	U	SMPL
K1846-08 - 1	TP-1-S	90	0.0021	-	7470A	PPB	13 Mar 2019 15:26:20	U	SMPL
K1846-12 - 1	TP-1-D	91	0.0023	-	7470A	PPB	13 Mar 2019 15:28:26	U	SMPL
CCV56 - 1	CCV56	21926	4.9240	-	7470A	PPB	13 Mar 2019 15:30:33	U	SMPL
CCB56 - 1	CCB56	-23	-0.0234	-	7470A	PPB	13 Mar 2019 15:32:39	U	SMPL
K1849-01 - 1	C1355-PC	88	0.0016	-	7470A	PPB	13 Mar 2019 15:34:46	U	SMPL
K1849-03 - 1	H1308-PC	78	-0.0006	-	7470A	PPB	13 Mar 2019 15:36:52	U	SMPL
K1849-05 - 1	PUMP-PC	82	0.0003	-	7470A	PPB	13 Mar 2019 15:38:59	U	SMPL
K1849-07 - 1	C135-CON	60	-0.0047	-	7470A	PPB	13 Mar 2019 15:41:06	U	SMPL
K1849-09 - 1	H1308-CON	80	-0.0002	-	7470A	PPB	13 Mar 2019 15:43:13	U	SMPL
K1849-11 - 1	PUMP-CON	37	-0.0099	-	7470A	PPB	13 Mar 2019 15:45:20	U	SMPL
K1849-13 - 1	WINDOW-GLASS	69	-0.0027	-	7470A	PPB	13 Mar 2019 15:47:27	U	SMPL
PB117878BL - 1	PBW	22	-0.0133	-	7470A	PPB	13 Mar 2019 15:49:35	U	SMPL
PB117878BS - 1	LCSW	17036	3.8218	-	7470A	PPB	13 Mar 2019 15:51:42	U	SMPL
K1844-03 - 1	DRUM-1-4	39	-0.0094	-	7470A	PPB	13 Mar 2019 15:53:49	U	SMPL
CCV57 - 1	CCV57	22120	4.9678	-	7470A	PPB	13 Mar 2019 15:55:55	U	SMPL
CCB57 - 1	CCB57	-41	-0.0275	-	7470A	PPB	13 Mar 2019 15:58:02	U	SMPL
K1844-03DUP - 1	DRUM-1-4DUP	40	-0.0092	-	7470A	PPB	13 Mar 2019 16:00:08	U	SMPL
K1844-03MS - 1	DRUM-1-4MS	17988	4.0364	-	7470A	PPB	13 Mar 2019 16:02:15	U	SMPL
K1844-03MSD - 1	DRUM-1-4MSD	17903	4.0172	-	7470A	PPB	13 Mar 2019 16:04:21	U	SMPL
PB117879BL - 1	PBW	-45	-0.0284	-	7470A	PPB	13 Mar 2019 16:06:27	U	SMPL
PB117879BS - 1	LCSW	17160	3.8498	-	7470A	PPB	13 Mar 2019 16:08:34	U	SMPL
K1856-02 - 1	BP-FW-MW01-20190310	-1	-0.0184	-	7470A	PPB	13 Mar 2019 16:10:41	U	SMPL
K1856-02DUP - 1	BP-FW-MW01-20190310DUP	18	-0.0142	-	7470A	PPB	13 Mar 2019 16:12:49	U	SMPL
K1856-02MS - 1	BP-FW-MW01-20190310MS	17108	3.8380	-	7470A	PPB	13 Mar 2019 16:14:56	U	SMPL
K1856-02MSD - 1	BP-FW-MW01-20190310MSD	16832	3.7758	-	7470A	PPB	13 Mar 2019 16:17:04	U	SMPL
K1856-03 - 1	BP-FW-MW02-20190310	21	-0.0135	-	7470A	PPB	13 Mar 2019 16:19:11	U	SMPL
CCV58 - 1	CCV58	22595	5.0748	-	7470A	PPB	13 Mar 2019 16:21:17	U	SMPL
CCB58 - 1	CCB58	-41	-0.0275	-	7470A	PPB	13 Mar 2019 16:23:23	U	SMPL
K1856-04 - 1	BP-FW-MW03-20190310	13	-0.0153	-	7470A	PPB	13 Mar 2019 16:25:30	U	SMPL
K1856-05 - 1	BP-HN-MW29D-20190310	14	-0.0151	-	7470A	PPB	13 Mar 2019 16:27:37	U	SMPL
K1856-06 - 1	BPS1-TT-MW301D-20190310	30	-0.0115	-	7470A	PPB	13 Mar 2019 16:29:43	U	SMPL
K1856-07 - 1	BPS1-TT-MW307D-20190311	38	-0.0097	-	7470A	PPB	13 Mar 2019 16:31:49	U	SMPL
K1856-08 - 1	BP-TT-AOC22-MW08-20190311	20	-0.0137	-	7470A	PPB	13 Mar 2019 16:33:56	U	SMPL
K1856-09 - 1	BP-TT-AOC22-MW09-20190311	96	0.0034	-	7470A	PPB	13 Mar 2019 16:36:03	U	SMPL
K1856-10 - 1	BP-TT-AOC22-MW07-20190311	46	-0.0079	-	7470A	PPB	13 Mar 2019 16:38:11	U	SMPL
K1856-11 - 1	BP-TT-AOC22-MW07-20190311-F	24	-0.0128	-	7470A	PPB	13 Mar 2019 16:40:19	U	SMPL
K1856-12 - 1	BPS1-TT-MW306D-20190311	17	-0.0144	-	7470A	PPB	13 Mar 2019 16:42:27	U	SMPL
K1856-13 - 1	BPS1-TT-MW302D-20190311	22	-0.0133	-	7470A	PPB	13 Mar 2019 16:44:34	U	SMPL
CCV59 - 1	CCV59	22178	4.9808	-	7470A	PPB	13 Mar 2019 16:46:41	U	SMPL
CCB59 - 1	CCB59	-18	-0.0223	-	7470A	PPB	13 Mar 2019 16:48:48	U	SMPL
PB117877TB - 1	PB117842TB	69	-0.0027	-	7470A	PPB	13 Mar 2019 16:50:55	U	SMPL
PB117878TB - 1	PB117845TB	92	0.0025	-	7470A	PPB	13 Mar 2019 16:53:02	U	SMPL
K1687-02LX5 - 1		27	-0.0121	-	7470A	PPB	13 Mar 2019 16:55:08	U	SMPL
K1687-02A - 1		17841	4.0033	-	7470A	PPB	13 Mar 2019 16:57:16	U	SMPL
K1844-03LX5 - 1		3	-0.0175	-	7470A	PPB	13 Mar 2019 16:59:23	U	SMPL
K1844-03A - 1		18109	4.0637	-	7470A	PPB	13 Mar 2019 17:01:30	U	SMPL
K1856-02LX5 - 1		-30	-0.0250	-	7470A	PPB	13 Mar 2019 17:03:37	U	SMPL
K1856-02A - 1		16832	3.7758	-	7470A	PPB	13 Mar 2019 17:05:46	U	SMPL
CCV60 - 1	CCV60	22486	5.0503	-	7470A	PPB	13 Mar 2019 17:07:55	U	SMPL
CCB60 - 1	CCB60	-32	-0.0254	-	7470A	PPB	13 Mar 2019 17:10:02	U	SMPL