

LB101551


7470A

INSTRUMENT ID: CU1

Linear

 μ Abs.:

42265

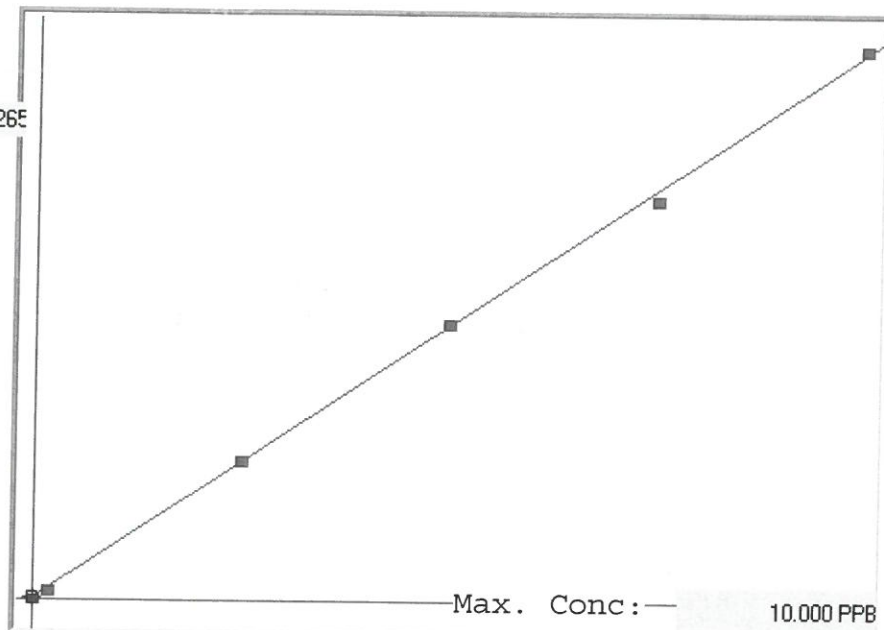

A= 0.0000e+000

B= 2.3932e-004

C= -2.6528e-002

Rho= 0.9997234

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.018	0.018	187	0.000	187				
0.2	0.200	0.163	-0.037	791	0.0 %	791				
2.5	2.500	2.556	0.056	10790	0.0 %	10790				
5.0	5.000	5.049	0.049	21208	0.0 %	21208				
7.5	7.500	7.326	-0.174	30724	0.0 %	30724				
10.0	10.000	10.088	0.088	42265	0.0 %	42265				

LB101551 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 22 Mar 2019 11:30:38

Sample ID	Extended ID	μ Abs	Conc	Std Cond Method	Units	Date	Type	Type
0.0 - 1	SC-0	187	-	0.00007470A	PPB	22 Mar 2019 12:16:09	S	Std
0.2 - 1	SC-2	791	-	0.20007470A	PPB	22 Mar 2019 12:18:17	S	Std
2.5 - 1	SC-5	10790	-	2.50007470A	PPB	22 Mar 2019 12:20:25	S	Std
5.0 - 1	SC-0	21208	-	5.00007470A	PPB	22 Mar 2019 12:22:33	S	Std
7.5 - 1	SC-5	30724	-	7.50007470A	PPB	22 Mar 2019 12:24:41	S	Std
10.0 - 1	SC-0	42265	-	10.00007470A	PPB	22 Mar 2019 12:31:23	S	Std
ICV65 - 1	ICV65	16470	3.9150	-7470A	PPB	22 Mar 2019 12:36:06	U	SMPL
ICB65 - 1	ICB65	151	0.0096	-7470A	PPB	22 Mar 2019 12:38:12	U	SMPL
CCV33 - 1	CCV33	21114	5.0264	-7470A	PPB	22 Mar 2019 12:40:18	U	SMPL
CCB33 - 1	CCB33	157	0.0110	-7470A	PPB	22 Mar 2019 12:42:24	U	SMPL
CRA - 1	CRA	775	0.1589	-7470A	PPB	22 Mar 2019 12:44:29	U	SMPL
HighStd - 1	HighStd	42323	10.1021	-7470A	PPB	22 Mar 2019 12:46:35	U	SMPL
ChkStd - 1	ChkStd	28522	6.7993	-7470A	PPB	22 Mar 2019 12:48:42	U	SMPL
PB118174BL - 1	PBW	-52	-0.0390	-7470A	PPB	22 Mar 2019 12:50:50	U	SMPL
PB118174BS - 1	LCSW	16839	4.0033	-7470A	PPB	22 Mar 2019 12:52:58	U	SMPL
K1690-02 - 1	HD-02-032019	153	0.0101	-7470A	PPB	22 Mar 2019 12:55:05	U	SMPL
K1690-02DUP - 1	HD-02-032019DUP	196	0.0204	-7470A	PPB	22 Mar 2019 12:57:13	U	SMPL
K1690-02MS - 1	HD-02-032019MS	16674	3.9638	-7470A	PPB	22 Mar 2019 12:59:21	U	SMPL
K1690-02MSD - 1	HD-02-032019MSD	16534	3.9303	-7470A	PPB	22 Mar 2019 13:01:29	U	SMPL
K1694-02 - 1	EO-02-032019-A	161	0.0120	-7470A	PPB	22 Mar 2019 13:03:36	U	SMPL
CCV34 - 1	CCV34	21428	5.1015	-7470A	PPB	22 Mar 2019 13:05:42	U	SMPL
CCB34 - 1	CCB34	26	-0.0203	-7470A	PPB	22 Mar 2019 13:07:48	U	SMPL
K1694-04 - 1	EO-02-032019-B	205	0.0225	-7470A	PPB	22 Mar 2019 13:09:55	U	SMPL
K1694-06 - 1	EO-02-032019-C	215	0.0249	-7470A	PPB	22 Mar 2019 13:12:01	U	SMPL
K1989-04 - 1	DRUM-1-2	197	0.0206	-7470A	PPB	22 Mar 2019 13:14:07	U	SMPL
K1994-04 - 1	50015-51054-30199-51048-51050	226	0.0276	-7470A	PPB	22 Mar 2019 13:16:14	U	SMPL
K2002-02 - 1	S-1(2-10)-COMP	254	0.0343	-7470A	PPB	22 Mar 2019 13:18:20	U	SMPL
K2002-04 - 1	S-2(5-30)-COMP	221	0.0264	-7470A	PPB	22 Mar 2019 13:20:28	U	SMPL
K2003-02 - 1	S4A(5-30)COMP	172	0.0146	-7470A	PPB	22 Mar 2019 13:22:35	U	SMPL
K2010-04 - 1	TP-1	195	0.0201	-7470A	PPB	22 Mar 2019 13:24:43	U	SMPL
K2036-09 - 1	WC-20190319	197	0.0206	-7470A	PPB	22 Mar 2019 13:26:51	U	SMPL
PB118189BL - 1	PBW	0	-0.0265	-7470A	PPB	22 Mar 2019 13:28:57	U	SMPL
CCV35 - 1	CCV35	21628	5.1494	-7470A	PPB	22 Mar 2019 13:31:04	U	SMPL
CCB35 - 1	CCB35	7	-0.0249	-7470A	PPB	22 Mar 2019 13:33:11	U	SMPL
PB118189BS - 1	LCSW	16960	4.0323	-7470A	PPB	22 Mar 2019 13:35:17	U	SMPL
K1832-08 - 1	PT-HG-WP	29532	7.0410	-7470A	PPB	22 Mar 2019 13:41:39	U	SMPL
PB118174TB - 1	PB118112TB	130	0.0046	-7470A	PPB	22 Mar 2019 13:43:46	U	SMPL
K1690-02LX5 - 1		26	-0.0203	-7470A	PPB	22 Mar 2019 13:45:54	U	SMPL
K1690-02A - 1		16843	4.0043	-7470A	PPB	22 Mar 2019 13:48:02	U	SMPL
CCV36 - 1	CCV36	21219	5.0515	-7470A	PPB	22 Mar 2019 13:50:10	U	SMPL
CCB36 - 1	CCB36	-21	-0.0316	-7470A	PPB	22 Mar 2019 13:52:20	U	SMPL