

213101570

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

3/22/2019 15:20

Test: Phenolics-

Sample Id	Result <i>mg/L</i>	Dil. 1 +	Response	Errors
ICV1	1.020	0.0	0.128	
ICB1	-0.002	0.0	0.018	
CCV1	0.986	0.0	0.124	
CCB1	-0.004	0.0	0.018	
PB118199BL	-0.002	0.0	0.018	
PB118199BS	1.001	0.0	0.126	
K1964-05	0.003	0.0	0.019	
K1964-05DUP	0.023	0.0	0.021	
K1964-05MS	1.022	0.0	0.128	
K1964-05MSD	1.018	0.0	0.128	
K2038-01	0.037	0.0	0.022	
CCV2	0.974	0.0	0.123	
CCB2	-0.004	0.0	0.018	

N	13
Mean	0.467
SD	0.5172
CV%	110.70

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

3/22/2019 14:55


Test Phenolics-

Accepted 3/22/2019 14:55

Factor 9.34
Bias 0.018

Coeff. of det. 0.999968

Errors

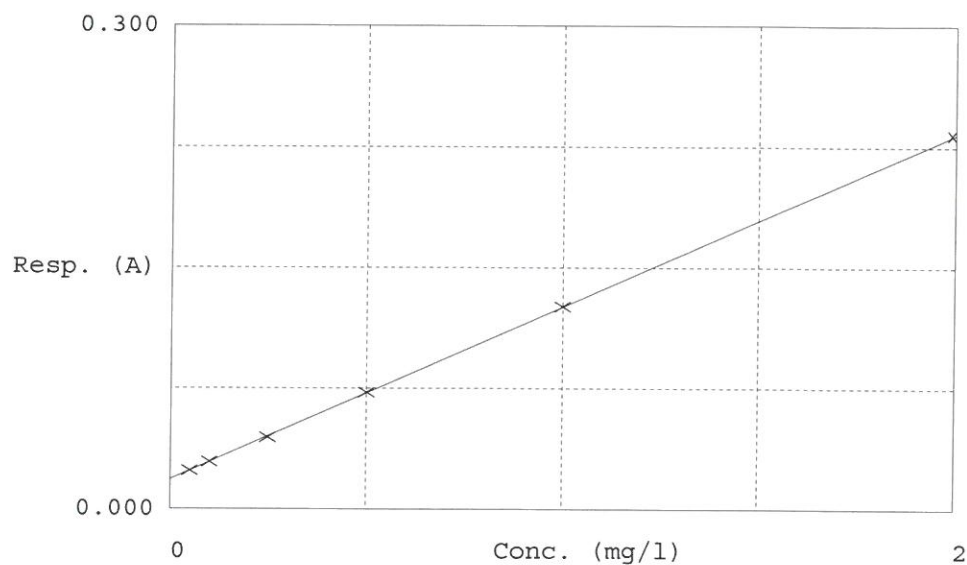

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.024	0.0504	0.0500	
2	Phenol-2	0.029	0.1015	0.1000	
3	Phenol-2	0.044	0.2425	0.2500	
4	Phenol-2	0.072	0.5044	0.5000	
5	Phenol-2	0.126	1.0028	1.0000	
6	Phenol-2	0.232	1.9983	2.0000	

AS

Aquakem v. 7.2AQ1

Results from time period:

Fri Mar 22 14:55:00 2019

Fri Mar 22 15:20:20 2019

Sample Id	Sam/Ctr/c/	Test short na	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0504	mg/l	3/22/2019 14:55:00	
0.1PPM	A	Phenolics-	P	0.1015	mg/l	3/22/2019 14:55:01	
0.25PPM	A	Phenolics-	P	0.2425	mg/l	3/22/2019 14:55:02	
0.50PPM	A	Phenolics-	P	0.5044	mg/l	3/22/2019 14:55:03	
1.0PPM	A	Phenolics-	P	1.0028	mg/l	3/22/2019 14:55:04	
2.0PPM	A	Phenolics-	P	1.9983	mg/l	3/22/2019 14:55:05	
ICV1	S	Phenolics-	P	1.0204	mg/l	3/22/2019 15:17:32	
ICB1	S	Phenolics-	P	-0.0016	mg/l	3/22/2019 15:17:33	
CCV1	S	Phenolics-	P	0.9856	mg/l	3/22/2019 15:17:34	
CCB1	S	Phenolics-	P	-0.0038	mg/l	3/22/2019 15:17:35	
PB118199BL	S	Phenolics-	P	-0.0024	mg/l	3/22/2019 15:17:36	
PB118199BS	S	Phenolics-	P	1.0012	mg/l	3/22/2019 15:17:37	
K1964-05	S	Phenolics-	P	0.0033	mg/l	3/22/2019 15:17:38	
K1964-05DUP	S	Phenolics-	P	0.0229	mg/l	3/22/2019 15:17:39	
K1964-05MS	S	Phenolics-	P	1.0222	mg/l	3/22/2019 15:17:40	
K1964-05MSD	S	Phenolics-	P	1.0183	mg/l	3/22/2019 15:17:41	
K2038-01	S	Phenolics-	P	0.037	mg/l	3/22/2019 15:17:42	
CCV2	S	Phenolics-	P	0.9741	mg/l	3/22/2019 15:17:43	
CCB2	S	Phenolics-	P	-0.0036	mg/l	3/22/2019 15:20:20	