

213/01605

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

3/25/2019 15:06

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.346	0.0	0.088	
ICB1	0.426	0.0	0.004	
CCV1	240.154	0.0	0.213	
CCB1	0.314	0.0	0.004	
PB118243BL	0.212	0.0	0.004	
PB118243BS	97.967	0.0	0.089	
MIDPB118243	243.531	0.0	0.216	
K1981-01	1.207	0.0	0.005	
K1981-01DUP	1.550	0.0	0.005	
K1981-01MS	31.653	0.0	0.031	
K1981-01MSD	31.458	0.0	0.031	
K1983-02	0.976	0.0	0.005	
CCV2	256.341	0.0	0.227	
CCB2	0.254	0.0	0.004	

N	14
Mean	71.599
SD	100.6893
CV%	140.63

Aquakem v. 7.2AQ1

Results from time period:

Mon Mar 25 14:52:20 2019

Mon Mar 25 14:56:13 2019

AB

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.0096	µg/l	3/25/2019 8:17:11	
5.OPPBCN	A	Total CN	P	4.2328	µg/l	3/25/2019 8:17:12	
10PPBCN	A	Total CN	P	10.0929	µg/l	3/25/2019 8:17:13	
50PPBCN	A	Total CN	P	50.1604	µg/l	3/25/2019 8:17:14	
100PPBCN	A	Total CN	P	101.5942	µg/l	3/25/2019 8:17:15	
250PPBCN	A	Total CN	P	248.4784	µg/l	3/25/2019 8:17:16	
500PPBCN	A	Total CN	P	500.4318	µg/l	3/25/2019 8:17:17	
ICV1	S	Total CN	P	96.3464	µg/l	3/25/2019 14:52:20	
ICB1	S	Total CN	P	0.4257	µg/l	3/25/2019 14:52:21	
CCV1	S	Total CN	P	240.1535	µg/l	3/25/2019 14:52:22	
CCB1	S	Total CN	P	0.3143	µg/l	3/25/2019 14:52:23	
PB118243BL	S	Total CN	P	0.2124	µg/l	3/25/2019 14:52:24	
PB118243BS	S	Total CN	P	97.9667	µg/l	3/25/2019 14:52:25	
MIDPB118243	S	Total CN	P	243.5307	µg/l	3/25/2019 14:52:26	
K1981-01	S	Total CN	P	1.207	µg/l	3/25/2019 14:52:27	
K1981-01DUP	S	Total CN	P	1.5501	µg/l	3/25/2019 14:52:28	
K1981-01MS	S	Total CN	P	31.6535	µg/l	3/25/2019 14:52:29	
K1981-01MSD	S	Total CN	P	31.4576	µg/l	3/25/2019 14:52:30	
K1983-02	S	Total CN	P	0.976	µg/l	3/25/2019 14:56:11	
CCV2	S	Total CN	P	256.341	µg/l	3/25/2019 14:56:12	
CCB2	S	Total CN	P	0.2536	µg/l	3/25/2019 14:56:13	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

3/25/2019 8:19


Test Total CN

Accepted 3/25/2019 8:19

Factor 1149
Bias 0.004

Coeff. of det. 0.999972

Errors

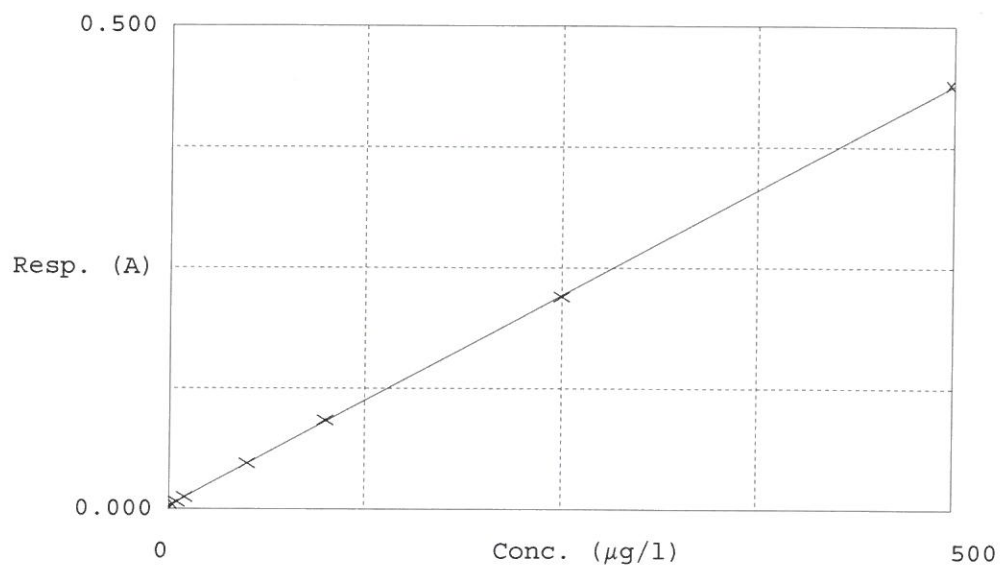

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.0096	0.0000	
2	5.0PPBCN	0.007	4.2328	5.0000	
3	10PPBCN	0.012	10.0929	10.0000	
4	50PPBCN	0.047	50.1604	50.0000	
5	100PPBCN	0.092	101.5942	100.0000	
6	250PPBCN	0.220	248.4784	250.0000	
7	500PPBCN	0.439	500.4318	500.0000	