

LB101631


7470A

INSTRUMENT ID: CU1

Linear

 μ Abs.:

41479

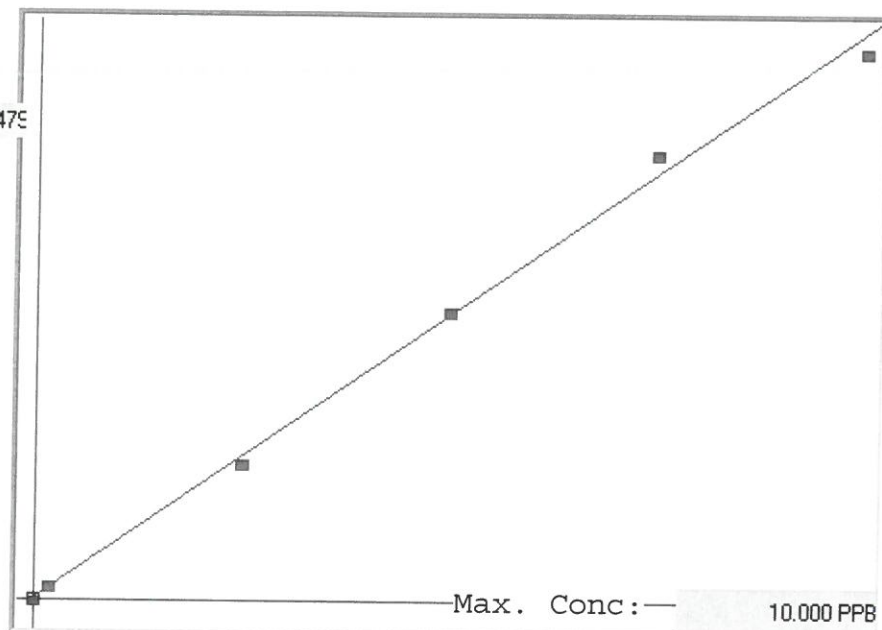

A= 0.0000e+000

B= 2.3431e-004

C= -2.3087e-002

Rho= 0.9984822

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.024	-0.024	-5	0.000	-5				
0.2	0.200	0.215	0.015	1014	0.0 %	1014				
2.5	2.500	2.380	-0.120	10254	0.0 %	10254				
5.0	5.000	5.066	0.066	21721	0.0 %	21721				
7.5	7.500	7.868	0.368	33679	0.0 %	33679				
10.0	10.000	9.696	-0.304	41479	0.0 %	41479				

LB101631 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 26 Mar 2019 14:01:41

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	-5	-	0.0000	7470A	PPB	26 Mar 2019 14:43:24	S	Std
0.2 - 1	50.2	1014	-	0.2000	7470A	PPB	26 Mar 2019 14:45:32	S	Std
2.5 - 1	52.5	10254	-	2.5000	7470A	PPB	26 Mar 2019 14:47:40	S	Std
5.0 - 1	55.0	21721	-	5.0000	7470A	PPB	26 Mar 2019 14:49:48	S	Std
7.5 - 1	57.5	33679	-	7.5000	7470A	PPB	26 Mar 2019 14:51:55	S	Std
10.0 - 1	510.0	41479	-	10.0000	7470A	PPB	26 Mar 2019 14:59:10	S	Std
ICV69 - 1	ICV69	17836	4.1560	-	7470A	PPB	26 Mar 2019 15:03:10	U	SMPL
ICB69 - 1	ICB69	60	-0.0090	-	7470A	PPB	26 Mar 2019 15:05:16	U	SMPL
CCV52 - 1	CCV52	21572	5.0314	-	7470A	PPB	26 Mar 2019 15:07:22	U	SMPL
CCB52 - 1	CCB52	63	-0.0083	-	7470A	PPB	26 Mar 2019 15:09:27	U	SMPL
CRA - 1	CRA	988	0.2084	-	7470A	PPB	26 Mar 2019 15:11:35	U	SMPL
HighStd - 1	HighStd	40445	9.4535	-	7470A	PPB	26 Mar 2019 15:13:41	U	SMPL
ChkStd - 1	ChkStd	31233	7.2951	-	7470A	PPB	26 Mar 2019 15:15:47	U	SMPL
PB118257BL - 1	PBW	-144	-0.0568	-	7470A	PPB	26 Mar 2019 15:17:55	U	SMPL
PB118257BS - 1	LCSW	17360	4.0445	-	7470A	PPB	26 Mar 2019 15:20:02	U	SMPL
K2040-02 - 1	S4B(2-10)	-80	-0.0418	-	7470A	PPB	26 Mar 2019 15:22:10	U	SMPL
K2040-02DUP - 1	S4B(2-10)DUP	-3	-0.0238	-	7470A	PPB	26 Mar 2019 15:24:17	U	SMPL
K2040-02MS - 1	S4B(2-10)MS	17016	3.9639	-	7470A	PPB	26 Mar 2019 15:26:25	U	SMPL
K2040-02MSD - 1	S4B(2-10)MSD	16774	3.9072	-	7470A	PPB	26 Mar 2019 15:28:33	U	SMPL
K2040-04 - 1	S4B(12-20)	-2	-0.0236	-	7470A	PPB	26 Mar 2019 15:30:39	U	SMPL
CCV53 - 1	CCV53	21504	5.0155	-	7470A	PPB	26 Mar 2019 15:32:45	U	SMPL
CCB53 - 1	CCB53	80	-0.0043	-	7470A	PPB	26 Mar 2019 15:34:51	U	SMPL
K2040-06 - 1	S4B(22-28)	1	-0.0229	-	7470A	PPB	26 Mar 2019 15:36:57	U	SMPL
K2050-07 - 1	CS-5	10	-0.0207	-	7470A	PPB	26 Mar 2019 15:39:03	U	SMPL
K2050-08 - 1	CS-4	12	-0.0203	-	7470A	PPB	26 Mar 2019 15:41:09	U	SMPL
K2050-09 - 1	CS-3	31	-0.0158	-	7470A	PPB	26 Mar 2019 15:43:16	U	SMPL
K2050-10 - 1	CS-2	23	-0.0177	-	7470A	PPB	26 Mar 2019 15:45:23	U	SMPL
K2050-11 - 1	CS-1	35	-0.0149	-	7470A	PPB	26 Mar 2019 15:47:31	U	SMPL
K2058-02 - 1	S3B(5-15)COMP	97	-0.0004	-	7470A	PPB	26 Mar 2019 15:49:38	U	SMPL
K2058-04 - 1	S3B(17-25)COMP	17	-0.0191	-	7470A	PPB	26 Mar 2019 15:51:46	U	SMPL
K2061-02 - 1	26524-27245	21	-0.0182	-	7470A	PPB	26 Mar 2019 15:53:54	U	SMPL
K2071-03 - 1	DRUM-1	56	-0.0100	-	7470A	PPB	26 Mar 2019 15:56:01	U	SMPL
CCV54 - 1	CCV54	21765	5.0766	-	7470A	PPB	26 Mar 2019 15:58:07	U	SMPL
CCB54 - 1	CCB54	112	0.0032	-	7470A	PPB	26 Mar 2019 16:00:14	U	SMPL
K2071-04 - 1	DRUM-2	16	-0.0193	-	7470A	PPB	26 Mar 2019 16:02:20	U	SMPL
PB118257TB - 1	PB118162TB	39	-0.0139	-	7470A	PPB	26 Mar 2019 16:04:27	U	SMPL
K2040-02LX5 - 1		-7	-0.0247	-	7470A	PPB	26 Mar 2019 16:06:33	U	SMPL
K2040-02A - 1		17380	4.0492	-	7470A	PPB	26 Mar 2019 16:08:40	U	SMPL
CCV55 - 1	CCV55	21768	5.0773	-	7470A	PPB	26 Mar 2019 16:10:47	U	SMPL
CCB55 - 1	CCB55	80	-0.0043	-	7470A	PPB	26 Mar 2019 16:12:54	U	SMPL