


LB101652

INSTRUMENT ID: CU1

7470A

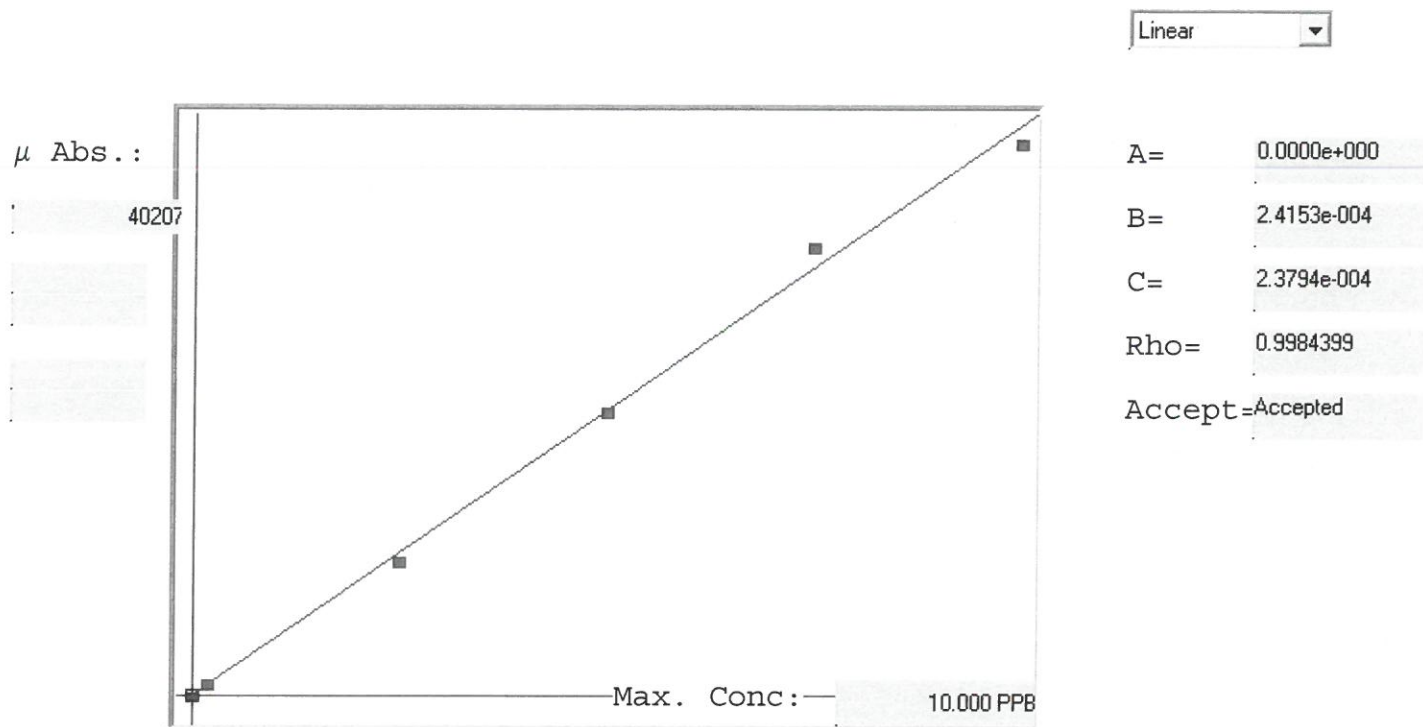

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.009	-0.009	-39	0.000	-39				
0.2	0.200	0.230	0.030	950	0.0 %	950				
2.5	2.500	2.381	-0.119	9858	0.0 %	9858				
5.0	5.000	4.992	-0.008	20666	0.0 %	20666				
7.5	7.500	7.895	0.395	32688	0.0 %	32688				
10.0	10.000	9.711	-0.289	40207	0.0 %	40207				

LB101652 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 27 Mar 2019 12:49:49

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1		-39	-	0.00007470A	PPB	27 Mar 2019 13:16:09	S	Std
0.2 - 1		950	-	0.20007470A	PPB	27 Mar 2019 13:18:17	S	Std
2.5 - 1		9858	-	2.50007470A	PPB	27 Mar 2019 13:20:26	S	Std
5.0 - 1		20666	-	5.00007470A	PPB	27 Mar 2019 13:22:34	S	Std
7.5 - 1		32688	-	7.50007470A	PPB	27 Mar 2019 13:24:41	S	Std
10.0 - 1		40207	-	10.00007470A	PPB	27 Mar 2019 13:32:34	S	Std
ICV71 - 1	ICV71	16402	3.9618	-7470A	PPB	27 Mar 2019 13:36:07	U	SMPL
ICB71 - 1	ICB71	79	0.0193	-7470A	PPB	27 Mar 2019 13:38:13	U	SMPL
CCV62 - 1	CCV62	20775	5.0180	-7470A	PPB	27 Mar 2019 13:40:19	U	SMPL
CCB62 - 1	CCB62	31	0.0077	-7470A	PPB	27 Mar 2019 13:42:25	U	SMPL
CRA - 1	CRA	929	0.2246	-7470A	PPB	27 Mar 2019 13:44:31	U	SMPL
HighStd - 1	HighStd	40143	9.6959	-7470A	PPB	27 Mar 2019 13:46:37	U	SMPL
ChkStd - 1	ChkStd	29689	7.1710	-7470A	PPB	27 Mar 2019 13:48:43	U	SMPL
PB118329BL - 1	PBW	233	0.0565	-7470A	PPB	27 Mar 2019 13:50:51	U	SMPL
PB118329BS - 1	LCSW	16834	4.0661	-7470A	PPB	27 Mar 2019 13:52:59	U	SMPL
K1693-14 - 1	OR-01-032519-A	755	0.1826	-7470A	PPB	27 Mar 2019 13:55:06	U	SMPL
K1693-14DUP - 1	OR-01-032519-ADUP	770	0.1862	-7470A	PPB	27 Mar 2019 13:57:13	U	SMPL
K1693-14MS - 1	OR-01-032519-AMS	17311	4.1813	-7470A	PPB	27 Mar 2019 13:59:21	U	SMPL
K1693-14MSD - 1	OR-01-032519-AMSD	17121	4.1354	-7470A	PPB	27 Mar 2019 14:01:30	U	SMPL
K1693-16 - 1	OR-01-032519-B	342	0.0828	-7470A	PPB	27 Mar 2019 14:03:35	U	SMPL
CCV63 - 1	CCV63	20673	4.9933	-7470A	PPB	27 Mar 2019 14:05:42	U	SMPL
CCB63 - 1	CCB63	0	0.0002	-7470A	PPB	27 Mar 2019 14:07:48	U	SMPL
K2081-02 - 1	S3A(2-10)	541	0.1309	-7470A	PPB	27 Mar 2019 14:09:54	U	SMPL
K2081-04 - 1	S3A(12-22)	901	0.2179	-7470A	PPB	27 Mar 2019 14:12:01	U	SMPL
K2081-15 - 1	S3A(22-28)-SB(27)COMP	747	0.1807	-7470A	PPB	27 Mar 2019 14:14:07	U	SMPL
K2081-17 - 1	S4C(6-18)COMP	116	0.0283	-7470A	PPB	27 Mar 2019 14:16:13	U	SMPL
K2081-19 - 1	S4C(18-29)COMP	280	0.0679	-7470A	PPB	27 Mar 2019 14:18:20	U	SMPL
K2091-02 - 1	DRUM-COMP	260	0.0630	-7470A	PPB	27 Mar 2019 14:20:27	U	SMPL
PB118329TB - 1	PB118253TB	658	0.1592	-7470A	PPB	27 Mar 2019 14:22:34	U	SMPL
K1693-14LX5 - 1		219	0.0531	-7470A	PPB	27 Mar 2019 14:24:42	U	SMPL
K1693-14A - 1		17204	4.1555	-7470A	PPB	27 Mar 2019 14:26:50	U	SMPL
CCV64 - 1	CCV64	20895	5.0470	-7470A	PPB	27 Mar 2019 14:28:56	U	SMPL
CCB64 - 1	CCB64	28	0.0070	-7470A	PPB	27 Mar 2019 14:31:02	U	SMPL