


LB101699

7471B

INSTRUMENT ID: CV1

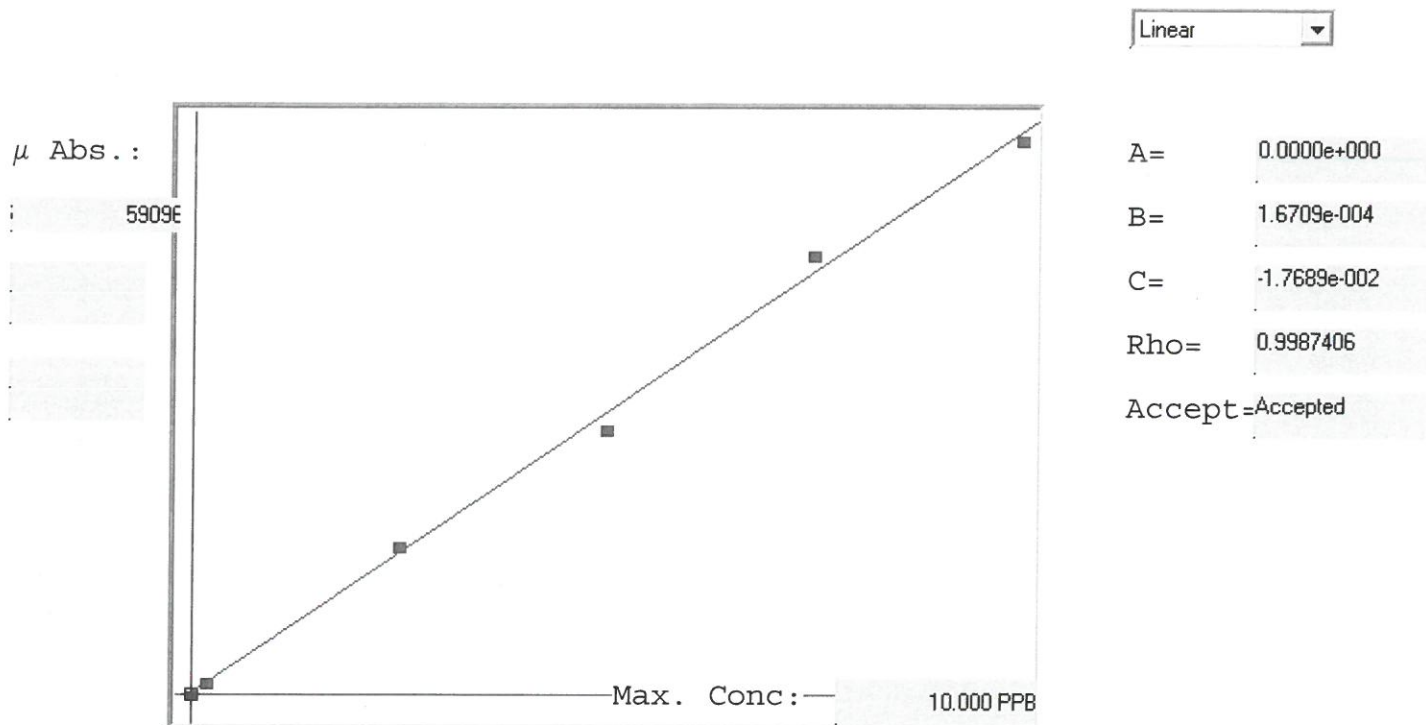

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.005	-0.005	73	0.000	73				
0.2	0.200	0.200	-0.000	1302	0.0 %	1302				
2.5	2.500	2.616	0.116	15762	0.0 %	15762				
5.0	5.000	4.724	-0.276	28377	0.0 %	28377				
7.5	7.500	7.809	0.309	46840	0.0 %	46840				
10.0	10.000	9.857	-0.143	59096	0.0 %	59096				

LB101699 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 28 Mar 2019 14:17:36

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50-0	73	-	0.00007471B	PPB	28 Mar 2019 15:04:12	S	Std
0.2 - 1	50-2	1302	-	0.20007471B	PPB	28 Mar 2019 15:06:29	S	Std
2.5 - 1	52-5	15762	-	2.50007471B	PPB	28 Mar 2019 15:08:46	S	Std
5.0 - 1	55-0	28377	-	5.00007471B	PPB	28 Mar 2019 15:11:03	S	Std
7.5 - 1	57-5	46840	-	7.50007471B	PPB	28 Mar 2019 15:13:20	S	Std
10.0 - 1	510-0	59096	-	10.00007471B	PPB	28 Mar 2019 15:23:50	S	Std
ICV74 - 1	ICV74	25906	4.3110	-7471B	PPB	28 Mar 2019 15:28:56	U	SMPL
ICB74 - 1	ICB74	43	-0.0105	-7471B	PPB	28 Mar 2019 15:31:11	U	SMPL
CCV74 - 1	CCV74	28428	4.7324	-7471B	PPB	28 Mar 2019 15:33:26	U	SMPL
CCB74 - 1	CCB74	-52	-0.0264	-7471B	PPB	28 Mar 2019 15:35:42	U	SMPL
CRA - 1	CRA	1297	0.1990	-7471B	PPB	28 Mar 2019 15:37:58	U	SMPL
HighStd - 1	HighStd	59281	9.8877	-7471B	PPB	28 Mar 2019 15:40:13	U	SMPL
ChkStd - 1	ChkStd	43127	7.1885	-7471B	PPB	28 Mar 2019 15:42:28	U	SMPL
PB118330BL - 1	PBS	-24	-0.0217	-7471B	PPB	28 Mar 2019 15:44:46	U	SMPL
PB118330BS - 1	LCSS	22573	3.7541	-7471B	PPB	28 Mar 2019 15:47:03	U	SMPL
K2086-01 - 1	CS-11	1432	0.2216	-7471B	PPB	28 Mar 2019 15:49:19	U	SMPL
K2086-02 - 1	CS-12	1292	0.1982	-7471B	PPB	28 Mar 2019 15:51:36	U	SMPL
K2086-03 - 1	CS-13	886	0.1304	-7471B	PPB	28 Mar 2019 15:53:53	U	SMPL
K2086-04 - 1	CS-14	843	0.1232	-7471B	PPB	28 Mar 2019 15:56:10	U	SMPL
K2086-05 - 1	CS-15	1315	0.2020	-7471B	PPB	28 Mar 2019 15:58:26	U	SMPL
CCV75 - 1	CCV75	31889	5.3107	-7471B	PPB	28 Mar 2019 16:00:41	U	SMPL
CCB75 - 1	CCB75	-22	-0.0214	-7471B	PPB	28 Mar 2019 16:02:56	U	SMPL
K2086-06 - 1	CS-16	567	0.0771	-7471B	PPB	28 Mar 2019 16:05:12	U	SMPL
K2086-07 - 1	CS-18	1130	0.1711	-7471B	PPB	28 Mar 2019 16:07:27	U	SMPL
K2090-02 - 1	P-5(0-10)	126062	21.0463	-7471B	PPB	28 Mar 2019 16:09:43	U	SMPL
K2102-01 - 1	TT-001-IDWSO-20190325	591	0.0811	-7471B	PPB	28 Mar 2019 16:11:59	U	SMPL
K2102-01DUP - 1	TT-001-IDWSO-20190325DUP	807	0.1172	-7471B	PPB	28 Mar 2019 16:14:16	U	SMPL
K2102-01MS - 1	TT-001-IDWSO-20190325MS	24473	4.0716	-7471B	PPB	28 Mar 2019 16:16:33	U	SMPL
K2102-01MSD - 1	TT-001-IDWSO-20190325MSD	24311	4.0445	-7471B	PPB	28 Mar 2019 16:18:49	U	SMPL
K2105-01 - 1	NJ-WATER	713	0.1014	-7471B	PPB	28 Mar 2019 16:21:07	U	SMPL
K2107-01 - 1	TP-1	4208	0.6854	-7471B	PPB	28 Mar 2019 16:23:24	U	SMPL
K2107-03 - 1	TP-2	2813	0.4523	-7471B	PPB	28 Mar 2019 16:25:40	U	SMPL
CCV76 - 1	CCV76	28560	4.7545	-7471B	PPB	28 Mar 2019 16:27:56	U	SMPL
CCB76 - 1	CCB76	-33	-0.0232	-7471B	PPB	28 Mar 2019 16:30:12	U	SMPL
K2107-05 - 1	TP-3	3072	0.4956	-7471B	PPB	28 Mar 2019 16:32:28	U	SMPL
K2107-07 - 1	TP-4	3036	0.4896	-7471B	PPB	28 Mar 2019 16:34:44	U	SMPL
K2107-09 - 1	TP-5	1857	0.2926	-7471B	PPB	28 Mar 2019 16:36:59	U	SMPL
K2107-11 - 1	TP-6	4164	0.6781	-7471B	PPB	28 Mar 2019 16:39:15	U	SMPL
K2107-13 - 1	TP-7	4982	0.8148	-7471B	PPB	28 Mar 2019 16:41:32	U	SMPL
K2107-15 - 1	TP-8	2425	0.3875	-7471B	PPB	28 Mar 2019 16:43:48	U	SMPL
K2107-17 - 1	TP-9	3262	0.5274	-7471B	PPB	28 Mar 2019 16:46:05	U	SMPL
PB118331BL - 1	PBS	111	0.0009	-7471B	PPB	28 Mar 2019 16:48:22	U	SMPL
PB118331BS - 1	LCSS	22968	3.8201	-7471B	PPB	28 Mar 2019 16:50:39	U	SMPL
K1697-13 - 1	SU-02-032719-A	1310	0.2012	-7471B	PPB	28 Mar 2019 16:52:55	U	SMPL
CCV77 - 1	CCV77	28277	4.7072	-7471B	PPB	28 Mar 2019 16:55:11	U	SMPL
CCB77 - 1	CCB77	-26	-0.0220	-7471B	PPB	28 Mar 2019 16:57:26	U	SMPL
K1697-13DUP - 1	SU-02-032719-ADUP	1362	0.2099	-7471B	PPB	28 Mar 2019 16:59:44	U	SMPL
K1697-13MS - 1	SU-02-032719-AMS	25007	4.1608	-7471B	PPB	28 Mar 2019 17:02:00	U	SMPL
K1697-13MSD - 1	SU-02-032719-AMSD	24822	4.1299	-7471B	PPB	28 Mar 2019 17:04:15	U	SMPL
K1697-15 - 1	SU-02-032719-B	1092	0.1648	-7471B	PPB	28 Mar 2019 17:06:31	U	SMPL
K2097-01 - 1	CS-20	29692	4.9436	-7471B	PPB	28 Mar 2019 17:08:47	U	SMPL
K2097-02 - 1	CS-21	10606	1.7545	-7471B	PPB	28 Mar 2019 17:11:04	U	SMPL
K2097-03 - 1	CS-22	3577	0.5800	-7471B	PPB	28 Mar 2019 17:13:21	U	SMPL
K2097-04 - 1	CS-19	13671	2.2666	-7471B	PPB	28 Mar 2019 17:15:38	U	SMPL
K2097-05 - 1	CS-17	3362	0.5441	-7471B	PPB	28 Mar 2019 17:17:55	U	SMPL
K2097-06 - 1	CS-6	822	0.1197	-7471B	PPB	28 Mar 2019 17:20:10	U	SMPL
CCV78 - 1	CCV78	29847	4.9695	-7471B	PPB	28 Mar 2019 17:22:26	U	SMPL
CCB78 - 1	CCB78	-49	-0.0259	-7471B	PPB	28 Mar 2019 17:24:42	U	SMPL
K2111-01 - 1	S5(5-15)COMP	682	0.0963	-7471B	PPB	28 Mar 2019 17:26:58	U	SMPL
K2111-03 - 1	S5(17-25)COMP	674	0.0949	-7471B	PPB	28 Mar 2019 17:29:14	U	SMPL
K2111-05 - 1	S7A(4-20)COMP	193	0.0146	-7471B	PPB	28 Mar 2019 17:31:30	U	SMPL
K2112-04 - 1	DR-WC-001	9453	1.5618	-7471B	PPB	28 Mar 2019 17:33:46	U	SMPL
K2125-03 - 1	SOIL-COMP	911	0.1345	-7471B	PPB	28 Mar 2019 17:36:02	U	SMPL
K2130-01 - 1	FK-GF-02-034-A	4469	0.7290	-7471B	PPB	28 Mar 2019 17:38:19	U	SMPL
K2130-03 - 1	FK-GF-02-034-B	4870	0.7961	-7471B	PPB	28 Mar 2019 17:40:35	U	SMPL
K2131-01 - 1	FK-GF-02-035-A	4917	0.8039	-7471B	PPB	28 Mar 2019 17:42:52	U	SMPL
K2131-03 - 1	FK-GF-02-035-B	3276	0.5297	-7471B	PPB	28 Mar 2019 17:45:09	U	SMPL
K2132-01 - 1	FK-GF-02-036-A	4666	0.7620	-7471B	PPB	28 Mar 2019 17:47:26	U	SMPL
CCV79 - 1	CCV79	29364	4.8888	-7471B	PPB	28 Mar 2019 17:49:42	U	SMPL
CCB79 - 1	CCB79	-21	-0.0212	-7471B	PPB	28 Mar 2019 17:51:58	U	SMPL
K2132-03 - 1	FK-GF-02-036-B	3886	0.6316	-7471B	PPB	28 Mar 2019 17:54:15	U	SMPL
PB118382BL - 1	PBS	121	0.0025	-7471B	PPB	28 Mar 2019 17:56:31	U	SMPL
PB118382BS - 1	LCSS	22947	3.8166	-7471B	PPB	28 Mar 2019 17:58:48	U	SMPL
K1560-01 - 1	LOD-MDL-SOIL-01-QT1-2019	382	0.0461	-7471B	PPB	28 Mar 2019 18:04:58	U	SMPL
K1560-02 - 1	LOQ-SOIL-02-QT1-2019	2153	0.3421	-7471B	PPB	28 Mar 2019 18:14:17	U	SMPL
K2102-01LX5 - 1		144	0.0064	-7471B	PPB	28 Mar 2019 18:16:33	U	SMPL
K2102-01A - 1		22428	3.7299	-7471B	PPB	28 Mar 2019 18:18:50	U	SMPL
K1697-13LX5 - 1		164	0.0097	-7471B	PPB	28 Mar 2019 18:21:07	U	SMPL
K1697-13A - 1		23582	3.9227	-7471B	PPB	28 Mar 2019 18:23:24	U	SMPL
K2090-02DLX5 - 1		23955	3.9850	-7471B	PPB	28 Mar 2019 18:25:40	U	SMPL
CCV80 - 1	CCV80	28901	4.8114	-7471B	PPB	28 Mar 2019 18:27:57	U	SMPL
CCB80 - 1	CCB80	-62	-0.0280	-7471B	PPB	28 Mar 2019 18:30:14	U	SMPL