

LB101709


7470A

INSTRUMENT ID : CU1

Linear

 μ Abs.:

41974

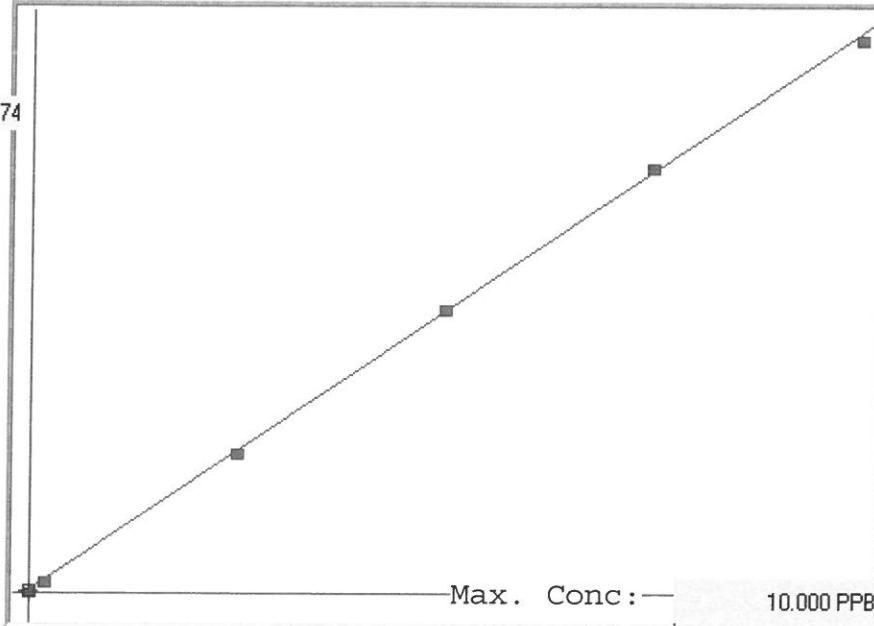

A= 0.0000e+000

B= 2.3668e-004

C= -4.9130e-002

Rho= 0.9998076

Accept = Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.011	-0.011	162	0.000	162				
0.2	0.200	0.165	-0.035	905	0.0 %	905				
2.5	2.500	2.484	-0.016	10704	0.0 %	10704				
5.0	5.000	5.064	0.064	21602	0.0 %	21602				
7.5	7.500	7.612	0.112	32371	0.0 %	32371				
10.0	10.000	9.885	-0.115	41974	0.0 %	41974				

LB101709 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 28 Mar 2019 18:51:38

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	162	-	0.0000	7470A	PPB	28 Mar 2019 18:51:45	S	Std
0.2 - 1	50.2	905	-	0.2000	7470A	PPB	28 Mar 2019 18:53:53	S	Std
2.5 - 1	52.5	10704	-	2.5000	7470A	PPB	28 Mar 2019 18:56:01	S	Std
5.0 - 1	55.0	21602	-	5.0000	7470A	PPB	28 Mar 2019 18:58:09	S	Std
7.5 - 1	57.5	32371	-	7.5000	7470A	PPB	28 Mar 2019 19:00:16	S	Std
10.0 - 1	510.0	41974	-	10.0000	7470A	PPB	28 Mar 2019 19:02:23	S	Std
ICV75 - 1	ICV75	18810	4.4028	-	7470A	PPB	28 Mar 2019 19:05:56	U	SMPL
ICB75 - 1	ICB75	0	-0.0491	-	7470A	PPB	28 Mar 2019 19:08:03	U	SMPL
ICV75 - 1	ICV75	16994	3.9730	-	7470A	PPB	28 Mar 2019 19:09:24	U	SMPL
ICB75 - 1	ICB75	92	-0.0274	-	7470A	PPB	28 Mar 2019 19:11:29	U	SMPL
CCV81 - 1	CCV81	21794	5.1091	-	7470A	PPB	28 Mar 2019 19:13:36	U	SMPL
CCB81 - 1	CCB81	6	-0.0477	-	7470A	PPB	28 Mar 2019 19:15:42	U	SMPL
CRA - 1	CRA	860	0.1544	-	7470A	PPB	28 Mar 2019 19:17:48	U	SMPL
HighStd - 1	HighStd	42209	9.9409	-	7470A	PPB	28 Mar 2019 19:19:54	U	SMPL
ChkStd - 1	ChkStd	30267	7.1145	-	7470A	PPB	28 Mar 2019 19:22:00	U	SMPL
PB118391BL - 1	PBW	-5	-0.0503	-	7470A	PPB	28 Mar 2019 19:24:08	U	SMPL
PB118391BS - 1	LCSW	19089	4.4689	-	7470A	PPB	28 Mar 2019 19:26:15	U	SMPL
K1560-07 - 1	LOD-MDL-WATER-01-QT1-2019	333	0.0297	-	7470A	PPB	28 Mar 2019 20:01:13	U	SMPL
K1560-08 - 1	LOQ-WATER-02-QT1-2019	1752	0.3655	-	7470A	PPB	28 Mar 2019 20:03:20	U	SMPL
CCV82 - 1	CCV82	21867	5.1264	-	7470A	PPB	28 Mar 2019 20:05:28	U	SMPL
CCB82 - 1	CCB82	-19	-0.0536	-	7470A	PPB	28 Mar 2019 20:07:36	U	SMPL