


LB101727

7470A

INSTRUMENT ID: CV1

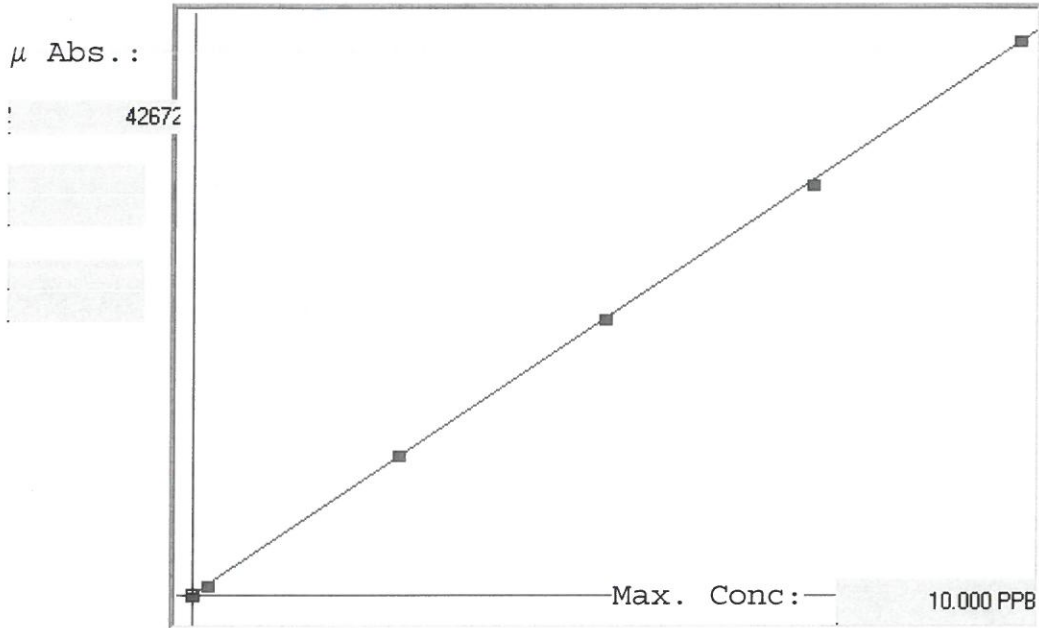

Linear

A= 0.0000e+000

B= 2.3530e-004

C= -9.9213e-003

Rho= 0.9999515

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.000	0.000	43	0.000	43				
0.2	0.200	0.177	-0.023	796	0.0 %	796				
2.5	2.500	2.541	0.041	10842	0.0 %	10842				
5.0	5.000	5.017	0.017	21364	0.0 %	21364				
7.5	7.500	7.433	-0.067	31632	0.0 %	31632				
10.0	10.000	10.031	0.031	42672	0.0 %	42672				

LB101727 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 29 Mar 2019 11:22:11

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc/Method	Units	Date	Type	Type
0.0 - 1	50.0	43	-	0.00007470A	PPB	29 Mar 2019 11:35:07	S	Std
0.2 - 1	50.2	796	-	0.20007470A	PPB	29 Mar 2019 11:37:15	S	Std
2.5 - 1	52.5	10842	-	2.50007470A	PPB	29 Mar 2019 11:39:23	S	Std
5.0 - 1	55.0	21364	-	5.00007470A	PPB	29 Mar 2019 11:41:31	S	Std
7.5 - 1	57.5	31632	-	7.50007470A	PPB	29 Mar 2019 11:43:39	S	Std
10.0 - 1	510.0	42672	-	10.00007470A	PPB	29 Mar 2019 11:45:45	S	Std
ICV77 - 1	ICV77	16516	3.8763	-7470A	PPB	29 Mar 2019 11:49:09	U	SMPL
ICB77 - 1	ICB77	-41	-0.0196	-7470A	PPB	29 Mar 2019 11:51:15	U	SMPL
CCV85 - 1	CCV85	21017	4.9354	-7470A	PPB	29 Mar 2019 11:53:21	U	SMPL
CCB85 - 1	CCB85	-34	-0.0179	-7470A	PPB	29 Mar 2019 11:55:27	U	SMPL
CRA - 1	CRA	771	0.1715	-7470A	PPB	29 Mar 2019 11:57:33	U	SMPL
HighStd - 1	HighStd	43039	10.1173	-7470A	PPB	29 Mar 2019 11:59:38	U	SMPL
ChkStd - 1	ChkStd	29354	6.8972	-7470A	PPB	29 Mar 2019 12:01:45	U	SMPL
PB118409BL - 1	PBW	-65	-0.0252	-7470A	PPB	29 Mar 2019 12:03:53	U	SMPL
PB118409BS - 1	LCSW	16474	3.8665	-7470A	PPB	29 Mar 2019 12:05:59	U	SMPL
K2093-01 - 1	30035-1	-27	-0.0163	-7470A	PPB	29 Mar 2019 12:08:06	U	SMPL
K2093-02 - 1	30091-30097-4	47	0.0011	-7470A	PPB	29 Mar 2019 12:10:14	U	SMPL
K2104-03 - 1	DRUM-1	35	-0.0017	-7470A	PPB	29 Mar 2019 12:12:21	U	SMPL
K2104-04 - 1	DRUM-2	25	-0.0040	-7470A	PPB	29 Mar 2019 12:14:29	U	SMPL
K2107-02 - 1	TP-1	24	-0.0043	-7470A	PPB	29 Mar 2019 12:16:35	U	SMPL
CCV86 - 1	CCV86	21278	4.9969	-7470A	PPB	29 Mar 2019 12:18:41	U	SMPL
CCB86 - 1	CCB86	-18	-0.0142	-7470A	PPB	29 Mar 2019 12:20:47	U	SMPL
K2107-04 - 1	TP-2	27	-0.0036	-7470A	PPB	29 Mar 2019 12:22:53	U	SMPL
K2107-06 - 1	TP-3	50	0.0018	-7470A	PPB	29 Mar 2019 12:24:59	U	SMPL
K2107-08 - 1	TP-4	85	0.0101	-7470A	PPB	29 Mar 2019 12:27:05	U	SMPL
K2107-10 - 1	TP-5	68	0.0061	-7470A	PPB	29 Mar 2019 12:29:12	U	SMPL
K2107-12 - 1	TP-6	46	0.0009	-7470A	PPB	29 Mar 2019 12:31:18	U	SMPL
K2107-14 - 1	TP-7	32	-0.0024	-7470A	PPB	29 Mar 2019 12:33:25	U	SMPL
K2107-16 - 1	TP-8	34	-0.0019	-7470A	PPB	29 Mar 2019 12:35:33	U	SMPL
K2107-18 - 1	TP-9	51	0.0021	-7470A	PPB	29 Mar 2019 12:37:41	U	SMPL
K2110-01 - 1	30036	70	0.0065	-7470A	PPB	29 Mar 2019 12:39:49	U	SMPL
K2111-02 - 1	S5(5-15)COMP	73	0.0073	-7470A	PPB	29 Mar 2019 12:41:55	U	SMPL
CCV87 - 1	CCV87	21448	5.0369	-7470A	PPB	29 Mar 2019 12:44:01	U	SMPL
CCB87 - 1	CCB87	-31	-0.0172	-7470A	PPB	29 Mar 2019 12:46:08	U	SMPL
K2111-04 - 1	S5(17-25)COMP	52	0.0023	-7470A	PPB	29 Mar 2019 12:48:14	U	SMPL
K2111-06 - 1	S7A(4-20)COMP	26	-0.0038	-7470A	PPB	29 Mar 2019 12:50:20	U	SMPL
K2112-01 - 1	EPH-4-8-WC-001	85	0.0101	-7470A	PPB	29 Mar 2019 12:52:27	U	SMPL
K2112-02 - 1	EPH-4-8-WC-002	123	0.0190	-7470A	PPB	29 Mar 2019 12:54:34	U	SMPL
K2112-03 - 1	DR-WC-001	54	0.0028	-7470A	PPB	29 Mar 2019 12:56:40	U	SMPL
K2112-03DUP - 1	DR-WC-001DUP	35	-0.0017	-7470A	PPB	29 Mar 2019 12:58:47	U	SMPL
K2112-03MS - 1	DR-WC-001MS	17439	4.0935	-7470A	PPB	29 Mar 2019 13:00:54	U	SMPL
K2112-03MSD - 1	DR-WC-001MSD	17397	4.0836	-7470A	PPB	29 Mar 2019 13:03:02	U	SMPL
PB118410BL - 1	PBW	-17	-0.0139	-7470A	PPB	29 Mar 2019 13:05:10	U	SMPL
PB118410BS - 1	LCSW	17290	4.0585	-7470A	PPB	29 Mar 2019 13:07:17	U	SMPL
CCV88 - 1	CCV88	21254	4.9912	-7470A	PPB	29 Mar 2019 13:09:23	U	SMPL
CCB88 - 1	CCB88	-32	-0.0175	-7470A	PPB	29 Mar 2019 13:11:30	U	SMPL
K2093-03 - 1	DL-2-COMP	98	0.0131	-7470A	PPB	29 Mar 2019 13:13:36	U	SMPL
K2093-18 - 1	30092-30093-5	29	-0.0031	-7470A	PPB	29 Mar 2019 13:15:43	U	SMPL
K2093-21 - 1	30099-30100-OW-6	46	0.0009	-7470A	PPB	29 Mar 2019 13:17:50	U	SMPL
K2110-02 - 1	BUR-COMP	62	0.0047	-7470A	PPB	29 Mar 2019 13:19:56	U	SMPL
K2124-02 - 1	SAMPLE-1	46	0.0009	-7470A	PPB	29 Mar 2019 13:22:03	U	SMPL
K2124-05 - 1	SAMPLE-2	45	0.0007	-7470A	PPB	29 Mar 2019 13:24:10	U	SMPL
K2124-05DUP - 1	SAMPLE-2DUP	55	0.0030	-7470A	PPB	29 Mar 2019 13:26:17	U	SMPL
K2124-05MS - 1	SAMPLE-2MS	16993	3.9886	-7470A	PPB	29 Mar 2019 13:28:25	U	SMPL
K2124-05MSD - 1	SAMPLE-2MSD	17320	4.0655	-7470A	PPB	29 Mar 2019 13:30:34	U	SMPL
PB118411BL - 1	PBW	-28	-0.0165	-7470A	PPB	29 Mar 2019 13:32:40	U	SMPL
CCV89 - 1	CCV89	21314	5.0053	-7470A	PPB	29 Mar 2019 13:34:47	U	SMPL
CCB89 - 1	CCB89	-26	-0.0160	-7470A	PPB	29 Mar 2019 13:36:54	U	SMPL
PB118411BS - 1	LCSW	17280	4.0561	-7470A	PPB	29 Mar 2019 13:39:02	U	SMPL
K1560-09 - 1	MDL-MDL-WATER-03-QT1-2019	208	0.0390	-7470A	PPB	29 Mar 2019 13:44:28	U	SMPL
PB118409TB - 1	PB118317TB	59	0.0040	-7470A	PPB	29 Mar 2019 13:46:35	U	SMPL
PB118410TB - 1	PB118321TB	34	-0.0019	-7470A	PPB	29 Mar 2019 13:48:42	U	SMPL
K2112-03LX5 - 1		5	-0.0087	-7470A	PPB	29 Mar 2019 13:50:48	U	SMPL
K2112-03A - 1		17675	4.1491	-7470A	PPB	29 Mar 2019 13:52:55	U	SMPL
K2124-05LX5 - 1		-26	-0.0160	-7470A	PPB	29 Mar 2019 13:55:02	U	SMPL
K2124-05A - 1		17319	4.0653	-7470A	PPB	29 Mar 2019 13:57:10	U	SMPL
CCV90 - 1	CCV90	21349	5.0136	-7470A	PPB	29 Mar 2019 13:59:18	U	SMPL
CCB90 - 1	CCB90	-41	-0.0196	-7470A	PPB	29 Mar 2019 14:01:26	U	SMPL
K2081-04 - 1		35	-0.0017	-7470A	PPB	29 Mar 2019 14:27:03	U	SMPL
CCV91 - 1	CCV91	21135	4.9632	-7470A	PPB	29 Mar 2019 14:29:10	U	SMPL
CCB91 - 1	CCB91	-49	-0.0215	-7470A	PPB	29 Mar 2019 14:31:17	U	SMPL