


LB101762

245.1

INSTRUMENT ID: CU1

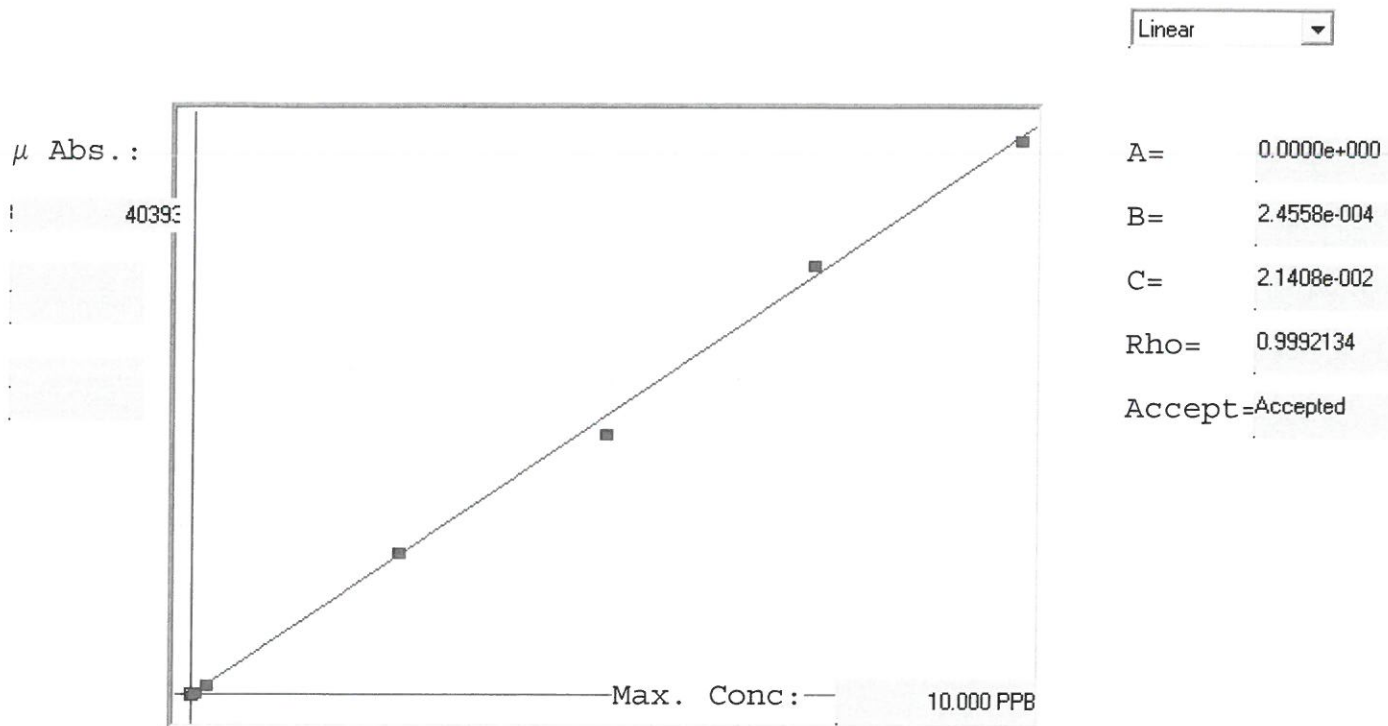

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.026	0.026	17	0.000	17				
0.05	0.050	0.061	0.011	160	0.0 %	160				
0.2	0.200	0.200	-0.000	727	0.0 %	727				
2.5	2.500	2.595	0.095	10480	0.0 %	10480				
5.0	5.000	4.703	-0.297	19064	0.0 %	19064				
7.5	7.500	7.724	0.224	31366	0.0 %	31366				
10.0	10.000	9.941	-0.059	40393	0.0 %	40393				

LB101762 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 29 Mar 2019 18:22:41

Sample ID	Extended ID	μ Abs.	Conc.	Std. Cond	Method	Units	Date	Type	Type
0.0 - 1	50.0	17	-	0.0000	245.1	PPB	29 Mar 2019 18:23:10	S	Std
0.05 - 1	50.05	160	-	0.0500	245.1	PPB	29 Mar 2019 18:25:28	S	Std
0.2 - 1	50.2	727	-	0.2000	245.1	PPB	29 Mar 2019 18:27:45	S	Std
2.5 - 1	52.5	10480	-	2.5000	245.1	PPB	29 Mar 2019 18:30:02	S	Std
5.0 - 1	55.0	19064	-	5.0000	245.1	PPB	29 Mar 2019 18:32:18	S	Std
7.5 - 1	57.5	31366	-	7.5000	245.1	PPB	29 Mar 2019 18:34:34	S	Std
10.0 - 1	510.0	40393	-	10.0000	245.1	PPB	29 Mar 2019 18:36:50	S	Std
ICV79 - 1	ICV79	15776	3.8957	-245.1		PPB	29 Mar 2019 18:40:33	U	SMPL
ICB79 - 1	ICB79	-67	0.0050	-245.1		PPB	29 Mar 2019 18:42:48	U	SMPL
CCV96 - 1	CCV96	19126	4.7184	-245.1		PPB	29 Mar 2019 18:45:04	U	SMPL
CCB96 - 1	CCB96	-45	0.0104	-245.1		PPB	29 Mar 2019 18:47:19	U	SMPL
CRA - 1	CRA	133	0.0541	-245.1		PPB	29 Mar 2019 18:49:34	U	SMPL
HighStd - 1	HighStd	40967	10.0821	-245.1		PPB	29 Mar 2019 18:51:49	U	SMPL
ChkStd - 1	ChkStd	28812	7.0971	-245.1		PPB	29 Mar 2019 18:54:04	U	SMPL
PB118415BL - 1	PBW	-99	-0.0029	-245.1		PPB	29 Mar 2019 18:56:23	U	SMPL
PB118415BS - 1	LCSW	15308	3.7808	-245.1		PPB	29 Mar 2019 18:58:39	U	SMPL
K1560-12 - 1	MDL-MDL-WATER-06-QT1-2019	129	0.0531	-245.1		PPB	29 Mar 2019 19:00:56	U	SMPL
CCV97 - 1	CCV97	19332	4.7690	-245.1		PPB	29 Mar 2019 19:03:12	U	SMPL
CCB97 - 1	CCB97	-77	0.0025	-245.1		PPB	29 Mar 2019 19:05:30	U	SMPL