

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/1/2019 14:43

Test: Total CN

Sample Id	Result <i>ug/d</i>	Dil. 1 +	Response	Errors
ICV1	97.935	0.0	0.091	
ICB1	0.358	0.0	0.004	
CCV1	241.298	0.0	0.219	
CCB1	0.342	0.0	0.004	
PB118470BL	0.354	0.0	0.004	
K1689-04	0.172	0.0	0.004	
K1689-04DUP	0.103	0.0	0.004	
K1689-06	0.321	0.0	0.004	
K1692-06	0.115	0.0	0.004	
K2171-02	0.421	0.0	0.004	
K2174-02	0.165	0.0	0.004	
K2179-04	0.501	0.0	0.005	
K2179-08	0.234	0.0	0.004	
K2179-12	0.203	0.0	0.004	
CCV2	245.959	0.0	0.223	
CCB2	0.404	0.0	0.004	
K2179-16	0.107	0.0	0.004	
K2179-20	0.158	0.0	0.004	
K2180-04	-0.106	0.0	0.004	
K2180-08	0.133	0.0	0.004	
K2180-12	0.181	0.0	0.004	
K2180-16	0.145	0.0	0.004	
K2180-20	0.813	0.0	0.005	
K2180-24	0.212	0.0	0.004	
K2180-28	0.259	0.0	0.004	
K2180-32	0.396	0.0	0.004	
CCV3	254.952	0.0	0.231	
CCB3	0.414	0.0	0.004	

N	28
Mean	30.234
SD	78.8154
CV%	260.69

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/1/2019 13:34


Test Total CN

Accepted 4/1/2019 13:34

Factor 1125
Bias 0.004

Coeff. of det. 0.999990

Errors

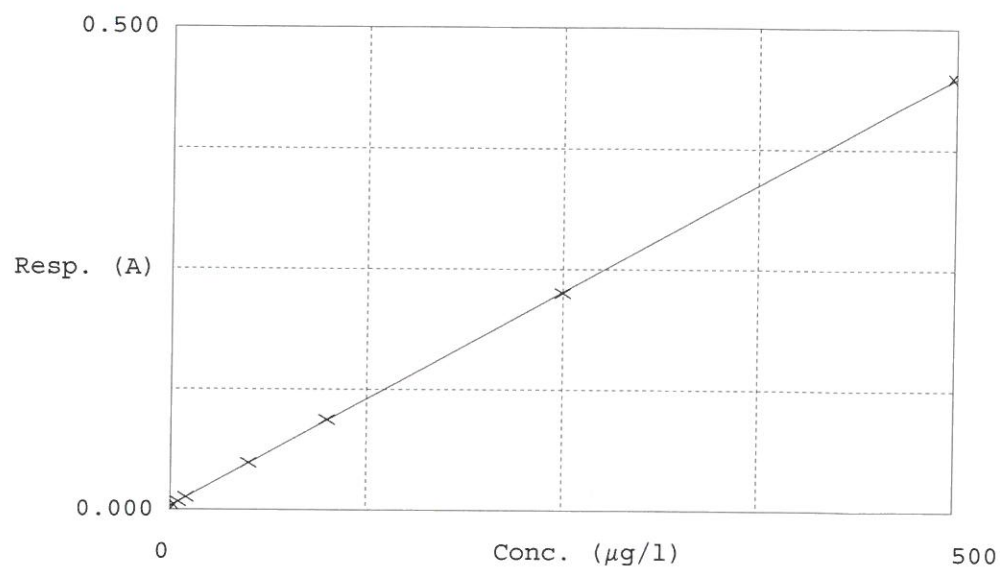

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.1311	0.0000	
2	5.0PPBCN	0.008	4.8585	5.0000	
3	10PPBCN	0.013	10.0486	10.0000	
4	50PPBCN	0.049	50.2417	50.0000	
5	100PPBCN	0.094	100.7257	100.0000	
6	250PPBCN	0.225	248.8511	250.0000	
7	500PPBCN	0.449	500.4056	500.0000	

AS

Aquakem v. 7.2AQ1

Results from time period:

Mon Apr 01 13:34:15 2019

Mon Apr 01 14:39:20 2019

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.1311	µg/l	4/1/2019 13:34:15	
5.OPPBCN	A	Reactive CN	P	4.8585	µg/l	4/1/2019 13:34:16	
10PPBCN	A	Reactive CN	P	10.0486	µg/l	4/1/2019 13:34:17	
50PPBCN	A	Reactive CN	P	50.2417	µg/l	4/1/2019 13:34:18	
100PPBCN	A	Reactive CN	P	100.7257	µg/l	4/1/2019 13:34:19	
250PPBCN	A	Reactive CN	P	248.8511	µg/l	4/1/2019 13:34:20	
500PPBCN	A	Reactive CN	P	500.4056	µg/l	4/1/2019 13:34:21	
ICV1	S	Reactive CN	P	97.9354	µg/l	4/1/2019 14:26:28	
ICB1	S	Reactive CN	P	0.3577	µg/l	4/1/2019 14:26:29	
CCV1	S	Reactive CN	P	241.2984	µg/l	4/1/2019 14:26:30	
CCB1	S	Reactive CN	P	0.3422	µg/l	4/1/2019 14:26:31	
PB118470BL	S	Reactive CN	P	0.3539	µg/l	4/1/2019 14:26:32	
K1689-04	S	Reactive CN	P	0.1716	µg/l	4/1/2019 14:26:33	
K1689-04DUP	S	Reactive CN	P	0.1033	µg/l	4/1/2019 14:26:34	
K1689-06	S	Reactive CN	P	0.3206	µg/l	4/1/2019 14:26:35	
K1692-06	S	Reactive CN	P	0.115	µg/l	4/1/2019 14:26:36	
K2171-02	S	Reactive CN	P	0.4207	µg/l	4/1/2019 14:26:37	
K2174-02	S	Reactive CN	P	0.1653	µg/l	4/1/2019 14:26:38	
K2179-04	S	Reactive CN	P	0.5008	µg/l	4/1/2019 14:34:00	
K2179-08	S	Reactive CN	P	0.2344	µg/l	4/1/2019 14:34:01	
K2179-12	S	Reactive CN	P	0.2033	µg/l	4/1/2019 14:34:02	
CCV2	S	Reactive CN	P	245.9587	µg/l	4/1/2019 14:34:03	
CCB2	S	Reactive CN	P	0.4041	µg/l	4/1/2019 14:34:04	
K2179-16	S	Reactive CN	P	0.1066	µg/l	4/1/2019 14:34:05	
K2179-20	S	Reactive CN	P	0.1584	µg/l	4/1/2019 14:34:06	
K2180-04	S	Reactive CN	P	-0.1062	µg/l	4/1/2019 14:34:07	
K2180-08	S	Reactive CN	P	0.1334	µg/l	4/1/2019 14:34:08	
K2180-12	S	Reactive CN	P	0.1805	µg/l	4/1/2019 14:34:09	
K2180-16	S	Reactive CN	P	0.1451	µg/l	4/1/2019 14:34:10	
K2180-20	S	Reactive CN	P	0.8129	µg/l	4/1/2019 14:39:15	
K2180-24	S	Reactive CN	P	0.2122	µg/l	4/1/2019 14:39:16	
K2180-28	S	Reactive CN	P	0.259	µg/l	4/1/2019 14:39:17	
K2180-32	S	Reactive CN	P	0.3955	µg/l	4/1/2019 14:39:18	
CCV3	S	Reactive CN	P	254.9518	µg/l	4/1/2019 14:39:19	
CCB3	S	Reactive CN	P	0.4145	µg/l	4/1/2019 14:39:20	