

2B101789

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/1/2019 15:30

Test: Total CN

Myld

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.566	0.0	0.091	
ICB1	0.543	0.0	0.005	
CCV1	243.816	0.0	0.221	
CCB1	0.365	0.0	0.004	
PB118469BL	0.409	0.0	0.004	
PB118469BS	98.836	0.0	0.092	
LOWPB118469	10.264	0.0	0.013	
HIGHPB118469	498.591	0.0	0.447	
K1689-03	4.192	0.0	0.008	
K1689-03DUP	3.857	0.0	0.007	
K1689-03MS	38.978	0.0	0.039	
K1689-03MSD	38.127	0.0	0.038	
K1689-05	3.300	0.0	0.007	
K1692-05	1.365	0.0	0.005	
CCV2	244.223	0.0	0.221	
CCB2	0.311	0.0	0.004	
K2171-01	0.455	0.0	0.004	
K2174-01	1.516	0.0	0.005	
K2179-03	0.466	0.0	0.004	
K2179-07	0.415	0.0	0.004	
K2179-11	0.711	0.0	0.005	
K2179-15	0.070	0.0	0.004	
K2179-19	0.150	0.0	0.004	
CCV3	260.091	0.0	0.235	
CCB3	0.279	0.0	0.004	

N	25
Mean	61.956
SD	122.7776
CV%	198.17

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/1/2019 13:34


Test Total CN

Accepted 4/1/2019 13:34

Factor 1125
Bias 0.004

Coeff. of det. 0.999990

Errors

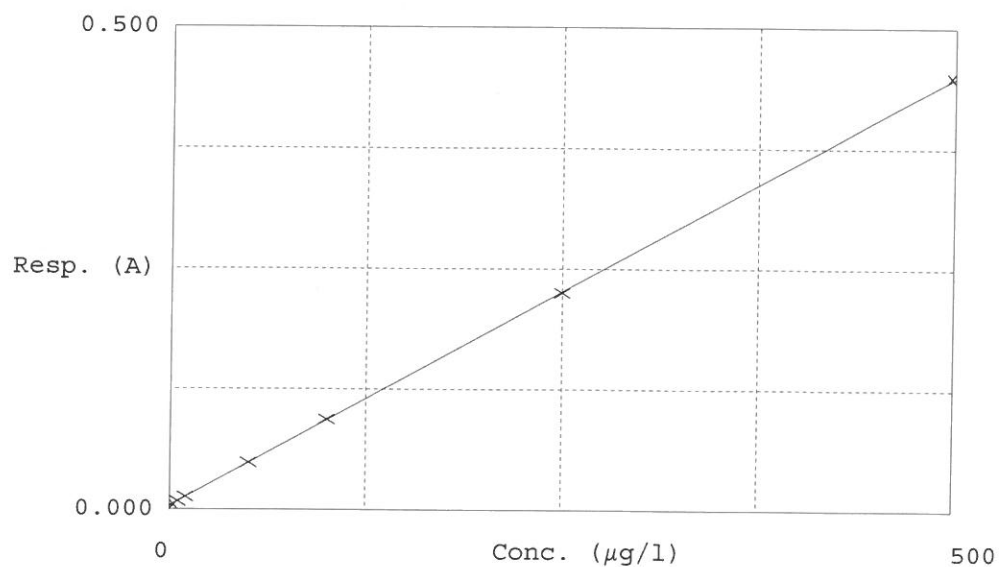

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.1311	0.0000	
2	5.0PPBCN	0.008	4.8585	5.0000	
3	10PPBCN	0.013	10.0486	10.0000	
4	50PPBCN	0.049	50.2417	50.0000	
5	100PPBCN	0.094	100.7257	100.0000	
6	250PPBCN	0.225	248.8511	250.0000	
7	500PPBCN	0.449	500.4056	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Mon Apr 01 15:18:20 2019

Mon Apr 01 15:29:48 2019

AS

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.1311	µg/l	4/1/2019 13:34:15	
5.0PPBCN	A	Total CN	P	4.8585	µg/l	4/1/2019 13:34:16	
10PPBCN	A	Total CN	P	10.0486	µg/l	4/1/2019 13:34:17	
50PPBCN	A	Total CN	P	50.2417	µg/l	4/1/2019 13:34:18	
100PPBCN	A	Total CN	P	100.7257	µg/l	4/1/2019 13:34:19	
250PPBCN	A	Total CN	P	248.8511	µg/l	4/1/2019 13:34:20	
500PPBCN	A	Total CN	P	500.4056	µg/l	4/1/2019 13:34:21	
ICV1	S	Total CN	P	97.5663	µg/l	4/1/2019 15:18:20	
ICB1	S	Total CN	P	0.5431	µg/l	4/1/2019 15:18:21	
CCV1	S	Total CN	P	243.8163	µg/l	4/1/2019 15:18:22	
CCB1	S	Total CN	P	0.3646	µg/l	4/1/2019 15:18:23	
PB118469BL	S	Total CN	P	0.4095	µg/l	4/1/2019 15:18:24	
PB118469BS	S	Total CN	P	98.8358	µg/l	4/1/2019 15:18:25	
LOWPB118469	S	Total CN	P	10.2643	µg/l	4/1/2019 15:18:26	
HIGHPB118469	S	Total CN	P	498.5911	µg/l	4/1/2019 15:18:27	
K1689-03	S	Total CN	P	4.1918	µg/l	4/1/2019 15:18:28	
K1689-03DUP	S	Total CN	P	3.8568	µg/l	4/1/2019 15:18:29	
K1689-03MS	S	Total CN	P	38.978	µg/l	4/1/2019 15:18:30	
K1689-03MSD	S	Total CN	P	38.1272	µg/l	4/1/2019 15:25:55	
K1689-05	S	Total CN	P	3.2996	µg/l	4/1/2019 15:25:56	
K1692-05	S	Total CN	P	1.3646	µg/l	4/1/2019 15:25:57	
CCV2	S	Total CN	P	244.2231	µg/l	4/1/2019 15:25:58	
CCB2	S	Total CN	P	0.3111	µg/l	4/1/2019 15:25:59	
K2171-01	S	Total CN	P	0.4548	µg/l	4/1/2019 15:26:00	
K2174-01	S	Total CN	P	1.516	µg/l	4/1/2019 15:26:01	
K2179-03	S	Total CN	P	0.4657	µg/l	4/1/2019 15:26:02	
K2179-07	S	Total CN	P	0.415	µg/l	4/1/2019 15:26:03	
K2179-11	S	Total CN	P	0.7114	µg/l	4/1/2019 15:26:04	
K2179-15	S	Total CN	P	0.0702	µg/l	4/1/2019 15:26:05	
K2179-19	S	Total CN	P	0.1502	µg/l	4/1/2019 15:29:46	
CCV3	S	Total CN	P	260.0909	µg/l	4/1/2019 15:29:47	
CCB3	S	Total CN	P	0.2787	µg/l	4/1/2019 15:29:48	