

LB101826


7470A

INSTRUMENT ID: CU1

Linear

 μ Abs.:

43479

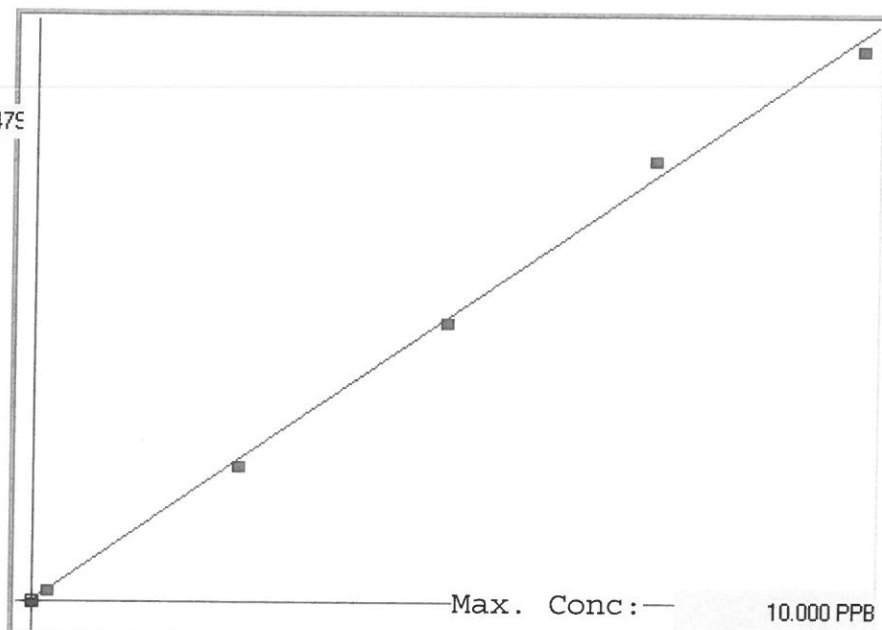

A= 0.0000e+000

B= 2.2512e-004

C= -1.0048e-002

Rho= 0.9989519

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.020	0.020	132	0.000	132				
0.2	0.200	0.199	-0.001	928	0.0 %	928				
2.5	2.500	2.423	-0.077	10808	0.0 %	10808				
5.0	5.000	4.945	-0.055	22009	0.0 %	22009				
7.5	7.500	7.836	0.336	34850	0.0 %	34850				
10.0	10.000	9.778	-0.222	43479	0.0 %	43479				

LB101826 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 03 Apr 2019 10:02:33

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	132	-	0.00007470A	PPB		03 Apr 2019 10:14:13	S	Std
0.2 - 1	50-2	928	-	0.20007470A	PPB		03 Apr 2019 10:16:21	S	Std
2.5 - 1	52-5	10808	-	2.50007470A	PPB		03 Apr 2019 10:18:30	S	Std
5.0 - 1	55-0	22009	-	5.00007470A	PPB		03 Apr 2019 10:20:38	S	Std
7.5 - 1	57-5	34850	-	7.50007470A	PPB		03 Apr 2019 10:22:45	S	Std
10.0 - 1	510-0	43479	-	10.00007470A	PPB		03 Apr 2019 10:28:23	S	Std
ICV84 - 1	ICV84	16750	3.7608	-7470A	PPB		03 Apr 2019 10:31:41	U	SMPL
ICB84 - 1	ICB84	85	0.0091	-7470A	PPB		03 Apr 2019 10:33:48	U	SMPL
CCV21 - 1	CCV21	22191	4.9857	-7470A	PPB		03 Apr 2019 10:35:53	U	SMPL
CCB21 - 1	CCB21	-10	-0.0123	-7470A	PPB		03 Apr 2019 10:37:59	U	SMPL
CRA - 1	CRA	939	0.2013	-7470A	PPB		03 Apr 2019 10:40:05	U	SMPL
HighStd - 1	HighStd	42913	9.6507	-7470A	PPB		03 Apr 2019 10:42:11	U	SMPL
ChkStd - 1	ChkStd	31675	7.1208	-7470A	PPB		03 Apr 2019 10:44:18	U	SMPL
PB118566BL - 1	PBW	13	-0.0071	-7470A	PPB		03 Apr 2019 10:46:25	U	SMPL
PB118566BS - 1	LCSW	16477	3.6993	-7470A	PPB		03 Apr 2019 10:48:32	U	SMPL
K1695-07 - 1	DPC-91723-SO-TP5-A	150	0.0237	-7470A	PPB		03 Apr 2019 10:50:40	U	SMPL
K1695-07DUP - 1	DPC-91723-SO-TP5-ADUP	182	0.0309	-7470A	PPB		03 Apr 2019 10:52:47	U	SMPL
K1695-07MS - 1	DPC-91723-SO-TP5-AMS	16753	3.7615	-7470A	PPB		03 Apr 2019 10:54:55	U	SMPL
K1695-07MSD - 1	DPC-91723-SO-TP5-AMSD	16470	3.6977	-7470A	PPB		03 Apr 2019 10:57:02	U	SMPL
K1695-11 - 1	DPC-91723-SO-TP5-B	144	0.0224	-7470A	PPB		03 Apr 2019 10:59:08	U	SMPL
CCV22 - 1	CCV22	22287	5.0073	-7470A	PPB		03 Apr 2019 11:01:14	U	SMPL
CCB22 - 1	CCB22	32	-0.0028	-7470A	PPB		03 Apr 2019 11:03:21	U	SMPL
K2185-03 - 1	P-4-OW(0-10)	179	0.0302	-7470A	PPB		03 Apr 2019 11:05:27	U	SMPL
K2190-03 - 1	VN-SP-1	149	0.0235	-7470A	PPB		03 Apr 2019 11:07:34	U	SMPL
K2190-06 - 1	VN-SP-2	167	0.0275	-7470A	PPB		03 Apr 2019 11:09:40	U	SMPL
K2196-02 - 1	HD-01-040119	163	0.0266	-7470A	PPB		03 Apr 2019 11:11:46	U	SMPL
K2213-02 - 1	S9A(2-10)COMP	188	0.0323	-7470A	PPB		03 Apr 2019 11:13:53	U	SMPL
K2213-04 - 1	S9A(12)-S9B(4)-S9B(8)-S9B(12)-S9C(12)	245	0.0451	-7470A	PPB		03 Apr 2019 11:16:00	U	SMPL
K2213-06 - 1	S9C(2-10)COMP	177	0.0298	-7470A	PPB		03 Apr 2019 11:18:08	U	SMPL
K2213-08 - 1	S10A(2-10)COMP	169	0.0280	-7470A	PPB		03 Apr 2019 11:20:15	U	SMPL
PB118568BL - 1	PBW	97	0.0118	-7470A	PPB		03 Apr 2019 11:22:23	U	SMPL
PB118568BS - 1	LCSW	16875	3.7889	-7470A	PPB		03 Apr 2019 11:24:30	U	SMPL
CCV23 - 1	CCV23	22327	5.0163	-7470A	PPB		03 Apr 2019 11:26:37	U	SMPL
CCB23 - 1	CCB23	46	0.0003	-7470A	PPB		03 Apr 2019 11:28:43	U	SMPL
K1695-02 - 1	SV-28399L	169	0.0280	-7470A	PPB		03 Apr 2019 11:30:50	U	SMPL
K1695-02DUP - 1	SV-28399LDUP	166	0.0273	-7470A	PPB		03 Apr 2019 11:32:56	U	SMPL
K1695-02MS - 1	SV-28399LMS	17351	3.8961	-7470A	PPB		03 Apr 2019 11:35:03	U	SMPL
K1695-02MSD - 1	SV-28399LMSD	17211	3.8646	-7470A	PPB		03 Apr 2019 11:37:09	U	SMPL
PB118566TB - 1	PB118499TB	135	0.0203	-7470A	PPB		03 Apr 2019 11:39:16	U	SMPL
PB118568TB - 1	PB118501TB	145	0.0226	-7470A	PPB		03 Apr 2019 11:41:23	U	SMPL
K1695-07LX5 - 1		-1	-0.0103	-7470A	PPB		03 Apr 2019 11:43:31	U	SMPL
K1695-07A - 1		16745	3.7597	-7470A	PPB		03 Apr 2019 11:45:39	U	SMPL
K1695-02LX5 - 1		-15	-0.0134	-7470A	PPB		03 Apr 2019 11:47:46	U	SMPL
K1695-02A - 1		17553	3.9416	-7470A	PPB		03 Apr 2019 11:49:53	U	SMPL
CCV24 - 1	CCV24	23815	5.3513	-7470A	PPB		03 Apr 2019 11:51:59	U	SMPL
CCB24 - 1	CCB24	21	-0.0053	-7470A	PPB		03 Apr 2019 11:54:05	U	SMPL