

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : AS

Instrument ID : Konelab

4/3/2019 14:59

Test: Total CN

mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	98.808	0.0	0.094	
ICB1	1.688	0.0	0.005	
CCV1	245.363	0.0	0.228	
CCB1	1.249	0.0	0.004	
PB118579BL	1.175	0.0	0.004	
PB118579BS	99.971	0.0	0.095	
LOWPB118579	11.352	0.0	0.014	
HIGHPB118579	495.116	0.0	0.457	
K2221-01	2.284	0.0	0.005	
K2221-01DUP	1.945	0.0	0.005	
K2221-01MS	13.483	0.0	0.016	
K2221-01MSD	13.431	0.0	0.016	
K2221-03	1.567	0.0	0.005	
K2230-01	1.405	0.0	0.005	
CCV2	247.118	0.0	0.230	
CCB2	1.167	0.0	0.004	
K2231-01	2.273	0.0	0.005	
K2232-01	2.130	0.0	0.005	
CCV3	243.614	0.0	0.226	
CCB3	1.268	0.0	0.004	

N	20
Mean	74.320
SD	132.8964
CV%	178.82

Aquakem v. 7.2AQ1

Results from time period:

Wed Apr 03 14:45:54 2019

Wed Apr 03 14:53:10 2019

AS

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.7302	µg/l	4/3/2019 8:03:09	
5.OPPBCN	A	Total CN	P	5.4303	µg/l	4/3/2019 8:03:10	
10PPBCN	A	Total CN	P	9.2007	µg/l	4/3/2019 8:03:11	
50PPBCN	A	Total CN	P	49.2089	µg/l	4/3/2019 8:03:12	
100PPBCN	A	Total CN	P	99.9098	µg/l	4/3/2019 8:03:13	
250PPBCN	A	Total CN	P	250.8227	µg/l	4/3/2019 8:03:14	
500PPBCN	A	Total CN	P	499.6975	µg/l	4/3/2019 8:03:15	
ICV1	S	Total CN	P	98.8075	µg/l	4/3/2019 14:45:54	
ICB1	S	Total CN	P	1.6882	µg/l	4/3/2019 14:45:55	
CCV1	S	Total CN	P	245.3633	µg/l	4/3/2019 14:45:56	
CCB1	S	Total CN	P	1.2485	µg/l	4/3/2019 14:45:57	
PB118579BL	S	Total CN	P	1.1747	µg/l	4/3/2019 14:45:58	
PB118579BS	S	Total CN	P	99.9707	µg/l	4/3/2019 14:45:59	
LOWPB118579	S	Total CN	P	11.3524	µg/l	4/3/2019 14:46:00	
HIGHPB118579	S	Total CN	P	495.1156	µg/l	4/3/2019 14:46:01	
K2221-01	S	Total CN	P	2.284	µg/l	4/3/2019 14:46:02	
K2221-01DUP	S	Total CN	P	1.9453	µg/l	4/3/2019 14:46:03	
K2221-01MS	S	Total CN	P	13.483	µg/l	4/3/2019 14:46:04	
K2221-01MSD	S	Total CN	P	13.4308	µg/l	4/3/2019 14:53:01	
K2221-03	S	Total CN	P	1.5671	µg/l	4/3/2019 14:53:02	
K2230-01	S	Total CN	P	1.4053	µg/l	4/3/2019 14:53:03	
CCV2	S	Total CN	P	247.1182	µg/l	4/3/2019 14:53:04	
CCB2	S	Total CN	P	1.1672	µg/l	4/3/2019 14:53:05	
K2231-01	S	Total CN	P	2.2731	µg/l	4/3/2019 14:53:06	
K2232-01	S	Total CN	P	2.1304	µg/l	4/3/2019 14:53:07	
CCV3	S	Total CN	P	243.6141	µg/l	4/3/2019 14:53:08	
CCB3	S	Total CN	P	1.2675	µg/l	4/3/2019 14:53:09	

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AS

Instrument ID : Konelab

4/3/2019 15:04


Test Total CN

Accepted 4/3/2019 9:21

Factor 1092
Bias 0.003

Coeff. of det. 0.999987

Errors

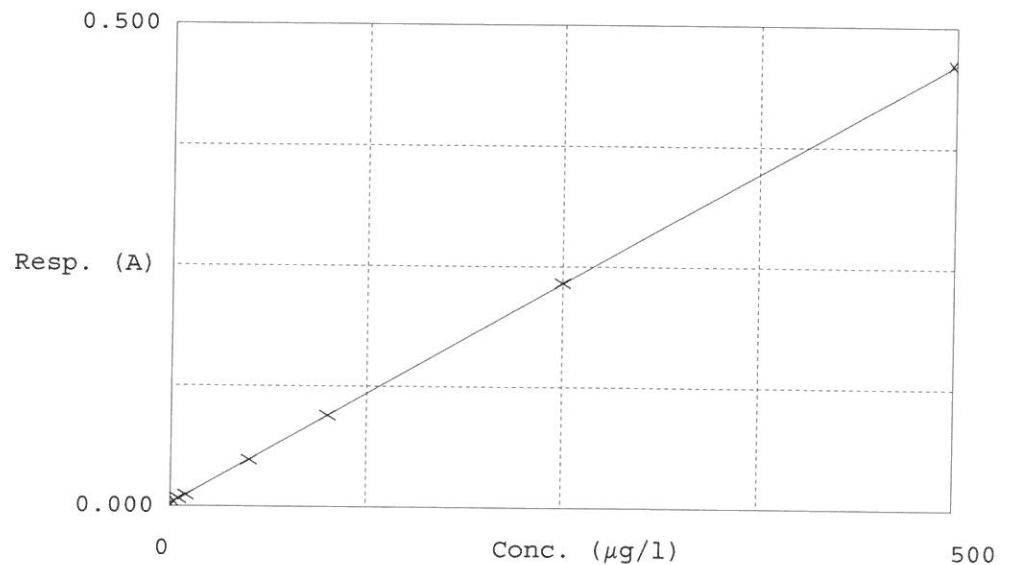

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.7302	0.0000	
2	5.0PPBCN	0.008	5.4303	5.0000	
3	10PPBCN	0.012	9.2007	10.0000	
4	50PPBCN	0.048	49.2089	50.0000	
5	100PPBCN	0.095	99.9098	100.0000	
6	250PPBCN	0.233	250.8227	250.0000	
7	500PPBCN	0.461	499.6975	500.0000	