

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/4/2019 15:14

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.648	0.0	0.091	
ICB1	-0.294	0.0	0.005	
CCV1	236.374	0.0	0.218	
CCB1	-0.315	0.0	0.004	
PB118619BL	-0.390	0.0	0.004	
PB118619BS	96.749	0.0	0.092	
MIDPB118619	237.739	0.0	0.219	
K2256-07	7.645	0.0	0.012	
K2256-07DUP	7.482	0.0	0.012	
K2256-07MS	46.023	0.0	0.046	
K2256-07MSD	45.311	0.0	0.046	
CCV2	253.070	0.0	0.233	
CCB2	-0.372	0.0	0.004	

N	13
Mean	78.821
SD	99.3590
CV%	126.06

Aquakem v. 7.2AQ1

Results from time period:

Thu Apr 04 15:06:26 2019

Thu Apr 04 15:09:50 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.5738	µg/l	4/4/2019 13:03:12	
5.0PPBCN	A	Total CN	P	4.3871	µg/l	4/4/2019 13:03:13	
10PPBCN	A	Total CN	P	9.6076	µg/l	4/4/2019 13:03:14	
50PPBCN	A	Total CN	P	49.5053	µg/l	4/4/2019 13:03:15	
100PPBCN	A	Total CN	P	101.1327	µg/l	4/4/2019 13:03:16	
250PPBCN	A	Total CN	P	252.2084	µg/l	4/4/2019 13:03:17	
500PPBCN	A	Total CN	P	498.7327	µg/l	4/4/2019 13:03:18	
ICV1	S	Total CN	P	95.648	µg/l	4/4/2019 15:06:26	
ICB1	S	Total CN	P	-0.2937	µg/l	4/4/2019 15:06:27	
CCV1	S	Total CN	P	236.3737	µg/l	4/4/2019 15:06:28	
CCB1	S	Total CN	P	-0.3147	µg/l	4/4/2019 15:06:29	
PB118619BL	S	Total CN	P	-0.39	µg/l	4/4/2019 15:06:30	
PB118619BS	S	Total CN	P	96.7493	µg/l	4/4/2019 15:06:31	
MIDPB118619	S	Total CN	P	237.7393	µg/l	4/4/2019 15:06:32	
K2256-07	S	Total CN	P	7.6453	µg/l	4/4/2019 15:06:33	
K2256-07DUP	S	Total CN	P	7.4821	µg/l	4/4/2019 15:06:34	
K2256-07MS	S	Total CN	P	46.0235	µg/l	4/4/2019 15:06:35	
K2256-07MSD	S	Total CN	P	45.3105	µg/l	4/4/2019 15:06:36	
CCV2	S	Total CN	P	253.0699	µg/l	4/4/2019 15:09:49	
CCB2	S	Total CN	P	-0.3725	µg/l	4/4/2019 15:09:50	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/4/2019 15:19


Test Total CN

Accepted 4/4/2019 13:05

Factor 1110
Bias 0.005

Coeff. of det. 0.999957

Errors

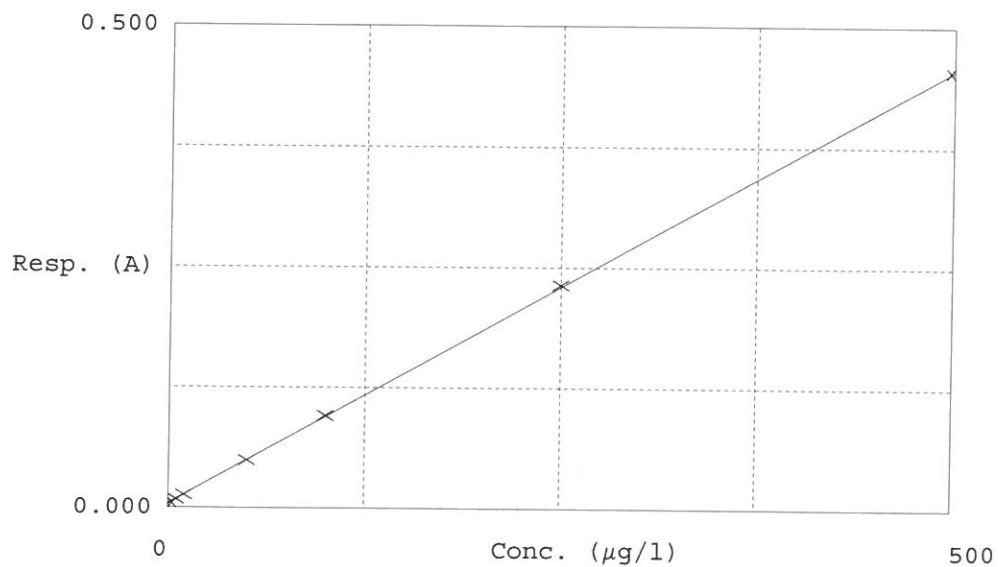

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.5738	0.0000	
2	5.0PPBCN	0.009	4.3871	5.0000	
3	10PPBCN	0.013	9.6076	10.0000	
4	50PPBCN	0.049	49.5053	50.0000	
5	100PPBCN	0.096	101.1327	100.0000	
6	250PPBCN	0.232	252.2084	250.0000	
7	500PPBCN	0.454	498.7327	500.0000	