


LB10/905

7470A

INSTRUMENT ID: CUI

Linear

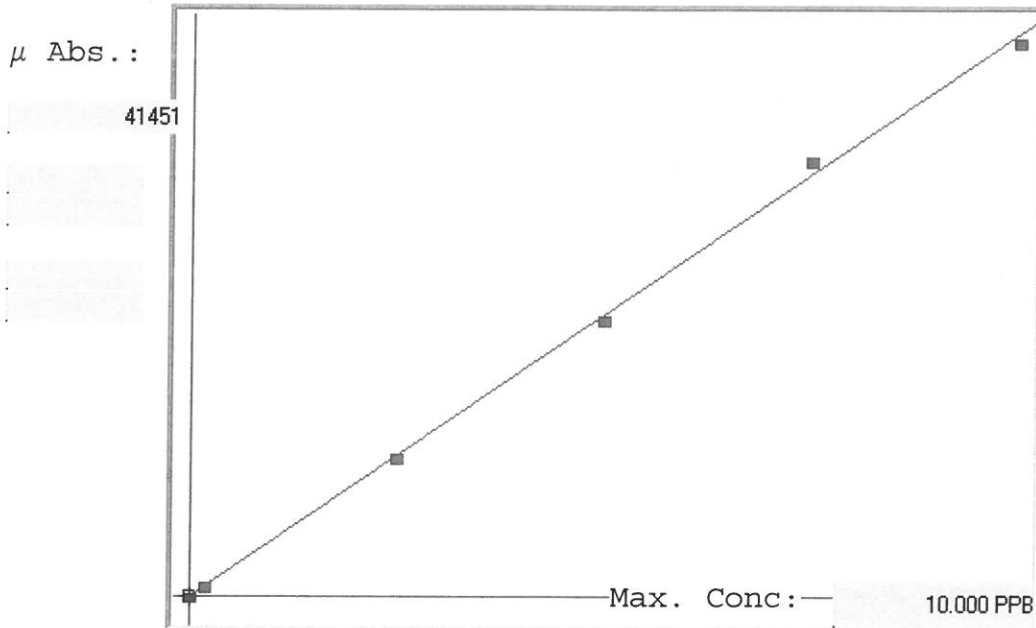

A= 0.0000e+000

B= 2.3734e-004

C= 1.0342e-002

Rho= 0.9994565

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.019	0.019	38	0.000	38				
0.2	0.200	0.185	-0.015	736	0.0 %	736				
2.5	2.500	2.467	-0.033	10351	0.0 %	10351				
5.0	5.000	4.935	-0.065	20751	0.0 %	20751				
7.5	7.500	7.745	0.245	32588	0.0 %	32588				
10.0	10.000	9.848	-0.152	41451	0.0 %	41451				

LB101905 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 05 Apr 2019 14:52:03

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	38	-	0.0000	7470A	PPB	05 Apr 2019 15:34:50	S	Std
0.2 - 1	50-2	736	-	0.2000	7470A	PPB	05 Apr 2019 15:36:58	S	Std
2.5 - 1	52-5	10351	-	2.5000	7470A	PPB	05 Apr 2019 15:39:06	S	Std
5.0 - 1	55-0	20751	-	5.0000	7470A	PPB	05 Apr 2019 15:41:14	S	Std
7.5 - 1	57-5	32588	-	7.5000	7470A	PPB	05 Apr 2019 15:43:21	S	Std
10.0 - 1	510-0	41451	-	10.0000	7470A	PPB	05 Apr 2019 15:48:48	S	Std
ICV91 - 1	ICV91	16565	3.9419	-	7470A	PPB	05 Apr 2019 15:52:03	U	SMPL
ICB91 - 1	ICB91	-25	0.0044	-	7470A	PPB	05 Apr 2019 15:54:10	U	SMPL
CCV51 - 1	CCV51	20698	4.9228	-	7470A	PPB	05 Apr 2019 15:56:15	U	SMPL
CCB51 - 1	CCB51	-50	-0.0015	-	7470A	PPB	05 Apr 2019 15:58:21	U	SMPL
CRA - 1	CRA	714	0.1798	-	7470A	PPB	05 Apr 2019 16:00:27	U	SMPL
HighStd - 1	HighStd	41774	9.9250	-	7470A	PPB	05 Apr 2019 16:02:33	U	SMPL
ChkStd - 1	ChkStd	29957	7.1204	-	7470A	PPB	05 Apr 2019 16:04:39	U	SMPL
PB118653BL - 1	PBW	-69	-0.0060	-	7470A	PPB	05 Apr 2019 16:06:47	U	SMPL
PB118653BS - 1	LCSW	15301	3.6419	-	7470A	PPB	05 Apr 2019 16:08:55	U	SMPL
K2222-07 - 1	VB-16206	-26	0.0042	-	7470A	PPB	05 Apr 2019 16:11:02	U	SMPL
K2265-02 - 1	BW-04419	-14	0.0070	-	7470A	PPB	05 Apr 2019 16:13:09	U	SMPL
K2265-02DUP - 1	BW-04419DUP	22	0.0156	-	7470A	PPB	05 Apr 2019 16:15:17	U	SMPL
K2265-02MS - 1	BW-04419MS	16596	3.9492	-	7470A	PPB	05 Apr 2019 16:17:25	U	SMPL
K2265-02MSD - 1	BW-04419MSD	16697	3.9732	-	7470A	PPB	05 Apr 2019 16:19:30	U	SMPL
CCV52 - 1	CCV52	20709	4.9254	-	7470A	PPB	05 Apr 2019 16:21:36	U	SMPL
CCB52 - 1	CCB52	-27	0.0039	-	7470A	PPB	05 Apr 2019 16:23:43	U	SMPL
PB118654BL - 1	PBW	20	0.0151	-	7470A	PPB	05 Apr 2019 16:25:52	U	SMPL
PB118654BS - 1	LCSW	15856	3.7736	-	7470A	PPB	05 Apr 2019 16:27:59	U	SMPL
K2240-17 - 1	SB-02-COMP	19	0.0149	-	7470A	PPB	05 Apr 2019 16:30:04	U	SMPL
K2240-19 - 1	SB-03-COMP	-1	0.0101	-	7470A	PPB	05 Apr 2019 16:32:12	U	SMPL
K2264-02 - 1	OPEN-WALL-EXCAVATION	16	0.0141	-	7470A	PPB	05 Apr 2019 16:34:18	U	SMPL
K2264-05 - 1	293-72-11966-238	18	0.0146	-	7470A	PPB	05 Apr 2019 16:36:25	U	SMPL
K2264-05DUP - 1	293-72-11966-238DUP	24	0.0160	-	7470A	PPB	05 Apr 2019 16:38:33	U	SMPL
K2264-05MS - 1	293-72-11966-238MS	16567	3.9424	-	7470A	PPB	05 Apr 2019 16:40:43	U	SMPL
K2264-05MSD - 1	293-72-11966-238MSD	16523	3.9319	-	7470A	PPB	05 Apr 2019 16:42:51	U	SMPL
PB118655BL - 1	PBW	11	0.0130	-	7470A	PPB	05 Apr 2019 16:44:57	U	SMPL
CCV53 - 1	CCV53	20616	4.9034	-	7470A	PPB	05 Apr 2019 16:47:04	U	SMPL
CCB53 - 1	CCB53	-51	-0.0018	-	7470A	PPB	05 Apr 2019 16:49:11	U	SMPL
PB118655BS - 1	LCSW	16669	3.9666	-	7470A	PPB	05 Apr 2019 16:51:17	U	SMPL
K2265-01 - 1	BW-04419	-17	0.0063	-	7470A	PPB	05 Apr 2019 16:53:24	U	SMPL
K2265-01DUP - 1	BW-04419DUP	27	0.0168	-	7470A	PPB	05 Apr 2019 16:55:30	U	SMPL
K2265-01MS - 1	BW-04419MS	17180	4.0879	-	7470A	PPB	05 Apr 2019 16:57:37	U	SMPL
K2265-01MSD - 1	BW-04419MSD	17082	4.0646	-	7470A	PPB	05 Apr 2019 16:59:44	U	SMPL
PB118664BL - 1	PBW	4	0.0113	-	7470A	PPB	05 Apr 2019 17:01:51	U	SMPL
PB118664BS - 1	LCSW	16086	3.8282	-	7470A	PPB	05 Apr 2019 17:03:58	U	SMPL
K2193-02 - 1	HR-06-040319-A	1	0.0106	-	7470A	PPB	05 Apr 2019 17:06:06	U	SMPL
K2193-02DUP - 1	HR-06-040319-ADUP	9	0.0125	-	7470A	PPB	05 Apr 2019 17:08:14	U	SMPL
K2193-02MS - 1	HR-06-040319-AMS	17001	4.0454	-	7470A	PPB	05 Apr 2019 17:10:21	U	SMPL
CCV54 - 1	CCV54	21379	5.0845	-	7470A	PPB	05 Apr 2019 17:12:27	U	SMPL
CCB54 - 1	CCB54	-37	0.0016	-	7470A	PPB	05 Apr 2019 17:14:33	U	SMPL
K2193-02MSD - 1	HR-06-040319-AMSD	17565	4.1792	-	7470A	PPB	05 Apr 2019 17:16:40	U	SMPL
K2193-04 - 1	HR-06-040319-B	3	0.0111	-	7470A	PPB	05 Apr 2019 17:18:46	U	SMPL
K2193-06 - 1	HR-06-040319-C	57	0.0239	-	7470A	PPB	05 Apr 2019 17:20:53	U	SMPL
K2195-02 - 1	NB-07-040319	62	0.0251	-	7470A	PPB	05 Apr 2019 17:22:59	U	SMPL
K2240-13 - 1	SB-01-COMP	53	0.0229	-	7470A	PPB	05 Apr 2019 17:25:06	U	SMPL
K2245-04 - 1	TP-1S	44	0.0208	-	7470A	PPB	05 Apr 2019 17:27:14	U	SMPL
K2245-08 - 1	TP-1D	22	0.0156	-	7470A	PPB	05 Apr 2019 17:29:21	U	SMPL
K2245-12 - 1	TP-3S	37	0.0191	-	7470A	PPB	05 Apr 2019 17:31:29	U	SMPL
K2245-16 - 1	TP-3D	135	0.0424	-	7470A	PPB	05 Apr 2019 17:33:37	U	SMPL
K2257-08 - 1	SP-1-A	59	0.0243	-	7470A	PPB	05 Apr 2019 17:35:44	U	SMPL
CCV55 - 1	CCV55	22644	5.3847	-	7470A	PPB	05 Apr 2019 17:37:50	U	SMPL
CCB55 - 1	CCB55	-27	0.0039	-	7470A	PPB	05 Apr 2019 17:39:57	U	SMPL
K2257-16 - 1	SP-1-B	37	0.0191	-	7470A	PPB	05 Apr 2019 17:42:04	U	SMPL
K2257-24 - 1	SP-1-C	31	0.0177	-	7470A	PPB	05 Apr 2019 17:44:10	U	SMPL
K2257-32 - 1	SP-1-D	79	0.0291	-	7470A	PPB	05 Apr 2019 17:46:16	U	SMPL
K2257-33 - 1	RO-20	53	0.0229	-	7470A	PPB	05 Apr 2019 17:48:23	U	SMPL
K2258-03 - 1	STONE	89	0.0315	-	7470A	PPB	05 Apr 2019 17:50:29	U	SMPL
PB118653TB - 1	PB118628TB	62	0.0251	-	7470A	PPB	05 Apr 2019 17:52:37	U	SMPL
PB118654TB - 1	PB118627TB	15	0.0139	-	7470A	PPB	05 Apr 2019 17:54:44	U	SMPL
PB118664TB - 1	PB118592TB	69	0.0267	-	7470A	PPB	05 Apr 2019 17:56:53	U	SMPL
K2265-02LX5 - 1		3	0.0111	-	7470A	PPB	05 Apr 2019 17:59:01	U	SMPL
K2265-02A - 1		16924	4.0271	-	7470A	PPB	05 Apr 2019 18:01:07	U	SMPL
CCV56 - 1	CCV56	22035	5.2401	-	7470A	PPB	05 Apr 2019 18:03:14	U	SMPL
CCB56 - 1	CCB56	-49	-0.0013	-	7470A	PPB	05 Apr 2019 18:05:22	U	SMPL
K2264-05LX5 - 1		-2	0.0099	-	7470A	PPB	05 Apr 2019 18:07:29	U	SMPL
K2264-05A - 1		16696	3.9730	-	7470A	PPB	05 Apr 2019 18:09:38	U	SMPL
K2265-01LX5 - 1		-24	0.0046	-	7470A	PPB	05 Apr 2019 18:11:45	U	SMPL
K2265-01A - 1		17281	4.1118	-	7470A	PPB	05 Apr 2019 18:13:53	U	SMPL
K2193-02LX5 - 1		-55	-0.0027	-	7470A	PPB	05 Apr 2019 18:16:02	U	SMPL
K2193-02A - 1		15756	3.7499	-	7470A	PPB	05 Apr 2019 18:18:09	U	SMPL
CCV57 - 1	CCV57	21011	4.9971	-	7470A	PPB	05 Apr 2019 18:20:16	U	SMPL
CCB57 - 1	CCB5	-54	-0.0025	-	7470A	PPB	05 Apr 2019 18:22:24	U	SMPL