

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/10/2019 15:57

Test: Phenolics-

mg/d

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.051	0.0	0.122	
ICB1	-0.003	0.0	0.013	
CCV1	1.044	0.0	0.122	
CCB1	-0.000	0.0	0.013	
PB118784BL	0.002	0.0	0.013	
PB118784BS	1.049	0.0	0.122	
K2241-12	0.007	0.0	0.014	
CCV2	1.049	0.0	0.122	
CCB2	0.001	0.0	0.013	

N	9
Mean	0.467
SD	0.5518
CV%	118.28

Aquakem v. 7.2AQ1

Results from time period:

Wed Apr 10 15:52:35 2019

Wed Apr 10 15:52:44 2019

AS

Sample Id	Sam/Ctr/c	Test short narr	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.051	mg/l	4/10/2019 14:56:41	
0.1PPM	A	Phenolics-	P	0.1001	mg/l	4/10/2019 14:56:42	
0.25PPM	A	Phenolics-	P	0.2496	mg/l	4/10/2019 14:56:43	
0.50PPM	A	Phenolics-	P	0.5016	mg/l	4/10/2019 14:56:44	
1.0PPM	A	Phenolics-	P	0.9963	mg/l	4/10/2019 14:56:45	
2.0PPM	A	Phenolics-	P	2.0015	mg/l	4/10/2019 14:56:46	
ICV1	S	Phenolics-	P	1.051	mg/l	4/10/2019 15:52:35	
ICB1	S	Phenolics-	P	-0.0027	mg/l	4/10/2019 15:52:36	
CCV1	S	Phenolics-	P	1.0444	mg/l	4/10/2019 15:52:37	
CCB1	S	Phenolics-	P	-0.0004	mg/l	4/10/2019 15:52:38	
PB118784BL	S	Phenolics-	P	0.0017	mg/l	4/10/2019 15:52:39	
PB118784BS	S	Phenolics-	P	1.0488	mg/l	4/10/2019 15:52:40	
K2241-12	S	Phenolics-	P	0.0068	mg/l	4/10/2019 15:52:41	
CCV2	S	Phenolics-	P	1.0487	mg/l	4/10/2019 15:52:43	
CCB2	S	Phenolics-	P	0.0007	mg/l	4/10/2019 15:52:44	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/10/2019 14:57


Test Phenolics-

Accepted 4/10/2019 14:57

Factor 9.615
Bias 0.013

Coeff. of det. 0.999993

Errors

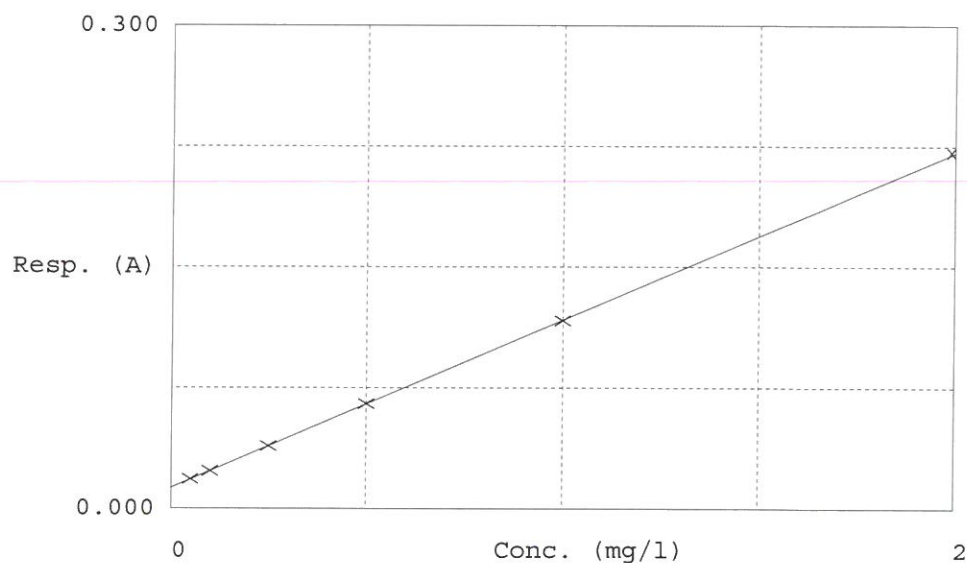

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.018	0.0510	0.0500	
2	Phenol-2	0.023	0.1001	0.1000	
3	Phenol-2	0.039	0.2496	0.2500	
4	Phenol-2	0.065	0.5016	0.5000	
5	Phenol-2	0.117	0.9963	1.0000	
6	Phenol-2	0.221	2.0015	2.0000	