

LB102032


7470A

INSTRUMENT ID: C01

Linear

 μ Abs.:

41771

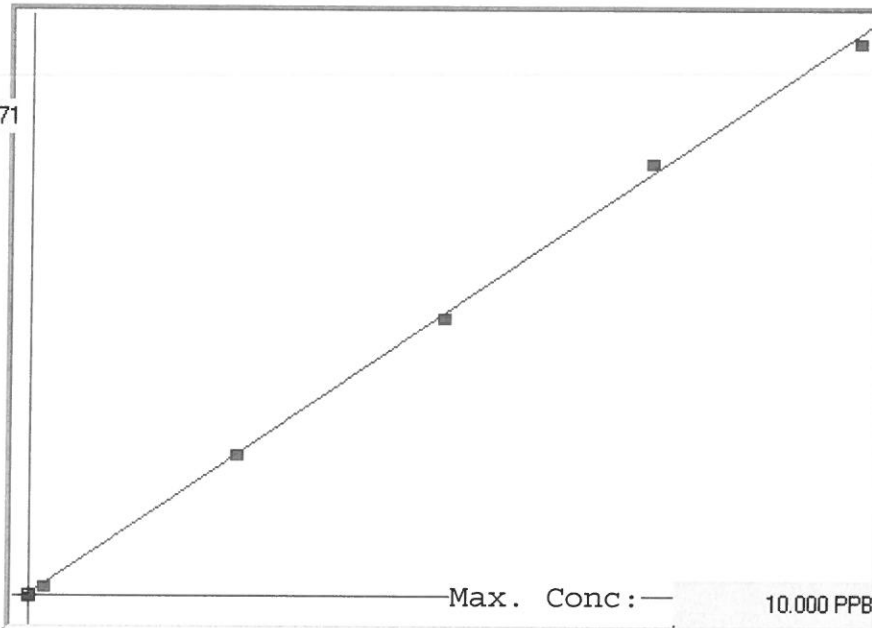

A= 0.0000e+000

B= 2.3631e-004

C= -1.7981e-002

Rho= 0.9995545

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.014	-0.014	17	0.000	17				
0.2	0.200	0.183	-0.017	849	0.0 %	849				
2.5	2.500	2.515	0.015	10717	0.0 %	10717				
5.0	5.000	4.946	-0.054	21004	0.0 %	21004				
7.5	7.500	7.718	0.218	32736	0.0 %	32736				
10.0	10.000	9.853	-0.147	41771	0.0 %	41771				

LB102032 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 11 Apr 2019 12:41:22

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	17	-	0.0000	7470A	PPB	11 Apr 2019 12:44:53	S	Std
0.2 - 1	50.2	849	-	0.2000	7470A	PPB	11 Apr 2019 12:47:01	S	Std
2.5 - 1	52.5	10717	-	2.5000	7470A	PPB	11 Apr 2019 12:49:09	S	Std
5.0 - 1	55.0	21004	-	5.0000	7470A	PPB	11 Apr 2019 12:51:17	S	Std
7.5 - 1	57.5	32736	-	7.5000	7470A	PPB	11 Apr 2019 12:53:25	S	Std
10.0 - 1	510.0	41771	-	10.0000	7470A	PPB	11 Apr 2019 13:06:57	S	Std
ICV95 - 1	ICV95	16905	3.9769	-	7470A	PPB	11 Apr 2019 13:09:34	U	SMPL
ICB95 - 1	ICB95	-44	-0.0284	-	7470A	PPB	11 Apr 2019 13:11:39	U	SMPL
CCV80 - 1	CCV80	21185	4.9883	-	7470A	PPB	11 Apr 2019 13:13:46	U	SMPL
CCB80 - 1	CCB80	-30	-0.0251	-	7470A	PPB	11 Apr 2019 13:15:51	U	SMPL
CRA - 1	CRA	822	0.1763	-	7470A	PPB	11 Apr 2019 13:17:57	U	SMPL
HighStd - 1	HighStd	41026	9.6771	-	7470A	PPB	11 Apr 2019 13:20:03	U	SMPL
ChkStd - 1	ChkStd	29710	7.0029	-	7470A	PPB	11 Apr 2019 13:22:10	U	SMPL
PB118816BL - 1	PBW	-19	-0.0225	-	7470A	PPB	11 Apr 2019 13:24:17	U	SMPL
PB118816BS - 1	LCSW	16558	3.8949	-	7470A	PPB	11 Apr 2019 13:26:24	U	SMPL
K2335-02 - 1	SV30755L	0	-0.0180	-	7470A	PPB	11 Apr 2019 13:28:31	U	SMPL
K2335-02DUP - 1	SV30755LDUP	29	-0.0111	-	7470A	PPB	11 Apr 2019 13:30:39	U	SMPL
K2335-02MS - 1	SV30755LMS	17064	4.0145	-	7470A	PPB	11 Apr 2019 13:32:47	U	SMPL
K2335-02MSD - 1	SV30755LMSD	17144	4.0334	-	7470A	PPB	11 Apr 2019 13:34:54	U	SMPL
K2342-18 - 1	TP-12	-3	-0.0187	-	7470A	PPB	11 Apr 2019 13:37:01	U	SMPL
CCV81 - 1	CCV81	20945	4.9316	-	7470A	PPB	11 Apr 2019 13:39:07	U	SMPL
CCB81 - 1	CCB81	-29	-0.0248	-	7470A	PPB	11 Apr 2019 13:41:13	U	SMPL
PB118817BL - 1	PBW	54	-0.0052	-	7470A	PPB	11 Apr 2019 13:43:19	U	SMPL
PB118817BS - 1	LCSW	16713	3.9315	-	7470A	PPB	11 Apr 2019 13:45:25	U	SMPL
K2200-02 - 1	EO-01-040919-A	46	-0.0071	-	7470A	PPB	11 Apr 2019 13:47:31	U	SMPL
K2200-02DUP - 1	EO-01-040919-ADUP	53	-0.0055	-	7470A	PPB	11 Apr 2019 13:49:38	U	SMPL
K2200-02MS - 1	EO-01-040919-AMS	18095	4.2581	-	7470A	PPB	11 Apr 2019 13:51:45	U	SMPL
K2200-02MSD - 1	EO-01-040919-AMSD	18265	4.2983	-	7470A	PPB	11 Apr 2019 13:53:53	U	SMPL
K2200-04 - 1	EO-01-040919-B	46	-0.0071	-	7470A	PPB	11 Apr 2019 13:56:00	U	SMPL
K2200-06 - 1	EO-01-040919-C	53	-0.0055	-	7470A	PPB	11 Apr 2019 13:58:08	U	SMPL
K2203-06 - 1	SU-04-040919-A	118	0.0099	-	7470A	PPB	11 Apr 2019 14:00:16	U	SMPL
K2203-08 - 1	SU-04-040919-B	100	0.0057	-	7470A	PPB	11 Apr 2019 14:02:22	U	SMPL
CCV82 - 1	CCV82	21117	4.9723	-	7470A	PPB	11 Apr 2019 14:04:29	U	SMPL
CCB82 - 1	CCB82	-36	-0.0265	-	7470A	PPB	11 Apr 2019 14:06:35	U	SMPL
K2334-03 - 1	P-6(0-10)	106	0.0071	-	7470A	PPB	11 Apr 2019 14:08:42	U	SMPL
K2342-04 - 1	TP-11-S	96	0.0047	-	7470A	PPB	11 Apr 2019 14:10:48	U	SMPL
K2342-08 - 1	TP-11-D	93	0.0040	-	7470A	PPB	11 Apr 2019 14:12:54	U	SMPL
K2342-12 - 1	TP-12-S	98	0.0052	-	7470A	PPB	11 Apr 2019 14:15:01	U	SMPL
K2342-16 - 1	TP-12-D	111	0.0083	-	7470A	PPB	11 Apr 2019 14:17:08	U	SMPL
K2343-04 - 1	TP-7-S	99	0.0054	-	7470A	PPB	11 Apr 2019 14:19:15	U	SMPL
K2343-08 - 1	TP-7-D	93	0.0040	-	7470A	PPB	11 Apr 2019 14:21:22	U	SMPL
K2344-03 - 1	WOOD-1	95	0.0045	-	7470A	PPB	11 Apr 2019 14:23:30	U	SMPL
K2344-05 - 1	WOOD-2	32	-0.0104	-	7470A	PPB	11 Apr 2019 14:25:38	U	SMPL
K2346-03 - 1	VNJ-229	28	-0.0114	-	7470A	PPB	11 Apr 2019 14:27:44	U	SMPL
CCV83 - 1	CCV83	21704	5.1110	-	7470A	PPB	11 Apr 2019 14:29:51	U	SMPL
CCB83 - 1	CCB83	-24	-0.0237	-	7470A	PPB	11 Apr 2019 14:31:58	U	SMPL
PB118818BL - 1	PBW	74	-0.0005	-	7470A	PPB	11 Apr 2019 14:34:04	U	SMPL
PB118818BS - 1	LCSW	16598	3.9044	-	7470A	PPB	11 Apr 2019 14:36:11	U	SMPL
K2311-01 - 1	0167-FIELD-BLANK	14	-0.0147	-	7470A	PPB	11 Apr 2019 14:38:17	U	SMPL
K2311-02 - 1	0168-SITE-WATER	129	0.0125	-	7470A	PPB	11 Apr 2019 14:40:24	U	SMPL
K2311-03 - 1	0236-COMP-CS-1-ELTRT	355	0.0659	-	7470A	PPB	11 Apr 2019 14:42:30	U	SMPL
K2311-04 - 1	0237-COMP-CS-2-ELTRT	236	0.0378	-	7470A	PPB	11 Apr 2019 14:44:37	U	SMPL
K2311-05 - 1	0238-COMP-CS-3-ELTRT	477	0.0947	-	7470A	PPB	11 Apr 2019 14:46:45	U	SMPL
K2311-06 - 1	0239-COMP-CS-4-ELTRT	176	0.0236	-	7470A	PPB	11 Apr 2019 14:48:53	U	SMPL
K2311-07 - 1	0240-COMP-CS-5-ELTRT	141	0.0153	-	7470A	PPB	11 Apr 2019 14:51:01	U	SMPL
K2311-07DUP - 1	0240-COMP-CS-5-ELTRTDUP	164	0.0208	-	7470A	PPB	11 Apr 2019 14:53:07	U	SMPL
CCV84 - 1	CCV84	21587	5.0833	-	7470A	PPB	11 Apr 2019 14:55:14	U	SMPL
CCB84 - 1	CCB84	-46	-0.0289	-	7470A	PPB	11 Apr 2019 14:57:20	U	SMPL
K2311-07MS - 1	0240-COMP-CS-5-ELTRTMS	19143	4.5058	-	7470A	PPB	11 Apr 2019 14:59:27	U	SMPL
K2311-07MSD - 1	0240-COMP-CS-5-ELTRTMSD	18975	4.4661	-	7470A	PPB	11 Apr 2019 15:01:33	U	SMPL
K2311-11 - 1	0236-COMP-CS-1-ELTRT-DISS	61	-0.0036	-	7470A	PPB	11 Apr 2019 15:03:40	U	SMPL
K2311-12 - 1	0239-COMP-CS-4-ELTRT-DISS	86	0.0023	-	7470A	PPB	11 Apr 2019 15:05:46	U	SMPL
K2311-13 - 1	0240-COMP-CS-5-ELTRT-DISS	78	0.0005	-	7470A	PPB	11 Apr 2019 15:07:54	U	SMPL
K2311-14 - 1	0237-COMP-CS-2-ELTRT-DISS	158	0.0194	-	7470A	PPB	11 Apr 2019 15:10:01	U	SMPL
K2311-15 - 1	0238-COMP-CS-3-ELTRT-DISS	253	0.0418	-	7470A	PPB	11 Apr 2019 15:12:08	U	SMPL
PB118816TB - 1	PB118757TB	14	-0.0147	-	7470A	PPB	11 Apr 2019 15:14:16	U	SMPL
PB118817TB - 1	PB118755TB	21	-0.0130	-	7470A	PPB	11 Apr 2019 15:16:24	U	SMPL
K2335-02LX5 - 1		1	-0.0177	-	7470A	PPB	11 Apr 2019 15:18:31	U	SMPL
CCV85 - 1	CCV85	21836	5.1422	-	7470A	PPB	11 Apr 2019 15:20:38	U	SMPL
CCB85 - 1	CCB85	-39	-0.0272	-	7470A	PPB	11 Apr 2019 15:22:45	U	SMPL
K2335-02A - 1		17174	4.0405	-	7470A	PPB	11 Apr 2019 15:24:52	U	SMPL
K2200-02LX5 - 1		-12	-0.0208	-	7470A	PPB	11 Apr 2019 15:26:59	U	SMPL
K2200-02A - 1		18306	4.3080	-	7470A	PPB	11 Apr 2019 15:29:06	U	SMPL
K2311-07LX5 - 1		17	-0.0140	-	7470A	PPB	11 Apr 2019 15:31:13	U	SMPL
K2311-07A - 1		19069	4.4883	-	7470A	PPB	11 Apr 2019 15:33:20	U	SMPL
CCV86 - 1	CCV86	21029	4.9515	-	7470A	PPB	11 Apr 2019 15:35:27	U	SMPL
CCB86 - 1	CCB86	-83	-0.0376	-	7470A	PPB	11 Apr 2019 15:37:35	U	SMPL