


LB102050

7471B

INSTRUMENT ID: CU1

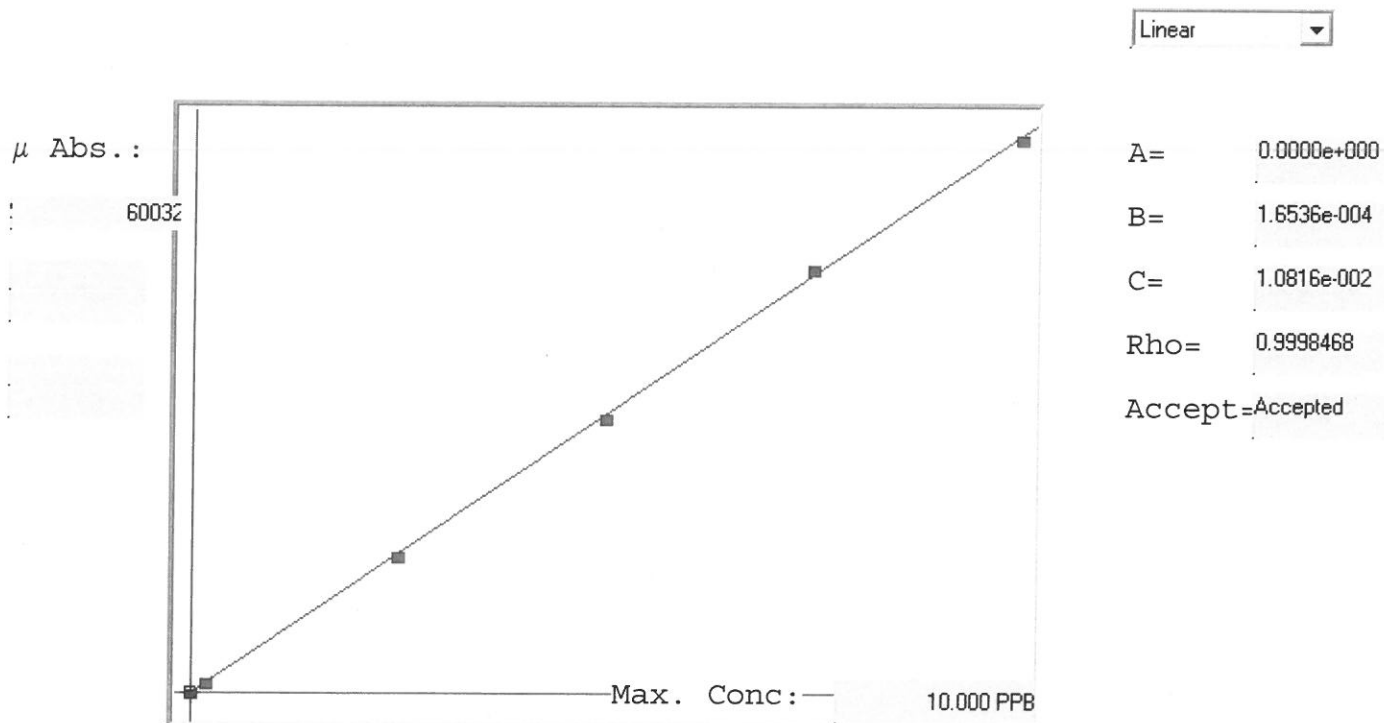

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.024	0.024	78	0.000	78				
0.2	0.200	0.200	0.000	1147	0.0 %	1147				
2.5	2.500	2.465	-0.035	14841	0.0 %	14841				
5.0	5.000	4.945	-0.055	29841	0.0 %	29841				
7.5	7.500	7.628	0.128	46064	0.0 %	46064				
10.0	10.000	9.938	-0.062	60032	0.0 %	60032				

LB102050 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 12 Apr 2019 10:48:21

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	78	-	0.0000	7471B	PPB	12 Apr 2019 10:57:03	S	Std
0.2 - 1	50-2	1147	-	0.2000	7471B	PPB	12 Apr 2019 10:59:20	S	Std
2.5 - 1	52-5	14841	-	2.5000	7471B	PPB	12 Apr 2019 11:01:37	S	Std
5.0 - 1	55-0	29841	-	5.0000	7471B	PPB	12 Apr 2019 11:03:54	S	Std
7.5 - 1	57-5	46064	-	7.5000	7471B	PPB	12 Apr 2019 11:06:10	S	Std
10.0 - 1	510-0	60032	-	10.0000	7471B	PPB	12 Apr 2019 11:11:48	S	Std
ICV97 - 1	ICV97	23913	3.9651	-	7471B	PPB	12 Apr 2019 11:14:40	U	SMPL
ICB97 - 1	ICB97	-19	0.0077	-	7471B	PPB	12 Apr 2019 11:16:56	U	SMPL
CCV90 - 1	CCV90	30197	5.0042	-	7471B	PPB	12 Apr 2019 11:19:11	U	SMPL
CCB90 - 1	CCB90	0	0.0108	-	7471B	PPB	12 Apr 2019 11:21:26	U	SMPL
CRA - 1	CRA	1143	0.1998	-	7471B	PPB	12 Apr 2019 11:23:42	U	SMPL
HighStd - 1	HighStd	60663	10.0420	-	7471B	PPB	12 Apr 2019 11:25:58	U	SMPL
ChkStd - 1	ChkStd	42570	7.0502	-	7471B	PPB	12 Apr 2019 11:28:13	U	SMPL
PB118854BL - 1	PBS	-103	-0.0062	-	7471B	PPB	12 Apr 2019 11:30:30	U	SMPL
PB118854BS - 1	LCSS	22046	3.6563	-	7471B	PPB	12 Apr 2019 11:32:47	U	SMPL
K2196-03 - 1	HD-02-041119	1498	0.2585	-	7471B	PPB	12 Apr 2019 11:35:04	U	SMPL
K2204-01 - 1	TR-04-041119	805	0.1439	-	7471B	PPB	12 Apr 2019 11:37:20	U	SMPL
K2355-03 - 1	TP-9-S	8170	1.3618	-	7471B	PPB	12 Apr 2019 11:39:37	U	SMPL
K2355-03DUP - 1	TP-9-SDUP	8165	1.3610	-	7471B	PPB	12 Apr 2019 11:41:54	U	SMPL
K2355-03MS - 1	TP-9-SMS	33539	5.5568	-	7471B	PPB	12 Apr 2019 11:44:09	U	SMPL
CCV91 - 1	CCV91	30732	5.0926	-	7471B	PPB	12 Apr 2019 11:46:25	U	SMPL
CCB91 - 1	CCB91	-58	0.0012	-	7471B	PPB	12 Apr 2019 11:48:41	U	SMPL
K2355-03MSD - 1	TP-9-SMSD	33427	5.5383	-	7471B	PPB	12 Apr 2019 11:50:57	U	SMPL
K2356-01 - 1	S-1	1901	0.3252	-	7471B	PPB	12 Apr 2019 11:53:13	U	SMPL
K2358-03 - 1	TP-5	70930	11.7397	-	7471B	PPB	12 Apr 2019 11:55:28	U	SMPL
K2358-07 - 1	TP-9	1939	0.3314	-	7471B	PPB	12 Apr 2019 11:57:44	U	SMPL
K2358-11 - 1	TP-7-S	228071	37.7245	-	7471B	PPB	12 Apr 2019 12:00:02	U	SMPL
K2358-15 - 1	TP-7-D	159238	26.3423	-	7471B	PPB	12 Apr 2019 12:02:18	U	SMPL
K2360-01 - 1	FK-BPM-01-E2-E2A-F2-F2A	465	0.0877	-	7471B	PPB	12 Apr 2019 12:04:37	U	SMPL
K2361-01 - 1	FK-BPM-01-E1-E1A-F1-F1A	1018	0.1792	-	7471B	PPB	12 Apr 2019 12:06:57	U	SMPL
K2373-01 - 1	TPH-FOUND	16268	2.7009	-	7471B	PPB	12 Apr 2019 12:09:14	U	SMPL
K2374-02 - 1	P-1(0-10)	735	0.1324	-	7471B	PPB	12 Apr 2019 12:11:30	U	SMPL
CCV92 - 1	CCV92	30708	5.0887	-	7471B	PPB	12 Apr 2019 12:13:46	U	SMPL
CCB92 - 1	CCB92	-35	0.0050	-	7471B	PPB	12 Apr 2019 12:16:02	U	SMPL
K2376-03 - 1	TP-4-S	227028	37.5520	-	7471B	PPB	12 Apr 2019 12:18:18	U	SMPL
K2377-03 - 1	TP-13-S	5353	0.8960	-	7471B	PPB	12 Apr 2019 12:20:34	U	SMPL
K2377-07 - 1	TP-12-S	9748	1.6227	-	7471B	PPB	12 Apr 2019 12:22:52	U	SMPL
K2355-03LX5 - 1		1616	0.2780	-	7471B	PPB	12 Apr 2019 12:25:08	U	SMPL
K2355-03A - 1		34078	5.6459	-	7471B	PPB	12 Apr 2019 12:27:23	U	SMPL
K2358-03DLX2 - 1		35736	5.9201	-	7471B	PPB	12 Apr 2019 12:29:40	U	SMPL
K2358-11DLX5 - 1		49085	8.1275	-	7471B	PPB	12 Apr 2019 12:31:57	U	SMPL
K2358-15DLX5 - 1		33103	5.4847	-	7471B	PPB	12 Apr 2019 12:34:14	U	SMPL
K2376-03DLX5 - 1		47429	7.8536	-	7471B	PPB	12 Apr 2019 12:36:33	U	SMPL
CCV93 - 1	CCV93	31029	5.1417	-	7471B	PPB	12 Apr 2019 12:38:50	U	SMPL
CCB93 - 1	CCB93	-51	0.0024	-	7471B	PPB	12 Apr 2019 12:41:06	U	SMPL