

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AS

Instrument ID : Konelab

4/15/2019 12:59

Test: Total CN

AS CCB2

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.824	0.0	0.093	
ICB1	0.567	0.0	0.004	
CCV1	239.478	0.0	0.228	
CCB12	0.254	0.0	0.004	
PB118886BL	0.260	0.0	0.004	
PB118886BS	95.521	0.0	0.093	
LOWPB118886	10.027	0.0	0.013	
HIGHPB118886	482.143	0.0	0.455	
K2199-09	1.239	0.0	0.005	
K2199-09DUP	0.448	0.0	0.004	
K2199-09MS	34.524	0.0	0.036	
K2199-09MSD	34.103	0.0	0.036	
K2199-11	1.142	0.0	0.005	
K2386-01	1.005	0.0	0.005	
CCV2	237.629	0.0	0.226	
CCB2	0.237	0.0	0.004	
K2390-01	0.497	0.0	0.004	
K2390-03	0.669	0.0	0.004	
K2390-05	0.596	0.0	0.004	
K2397-03	1.636	0.0	0.005	
K2397-07	5.390	0.0	0.009	
K2397-11	3.020	0.0	0.007	
K2397-15	1.568	0.0	0.005	
K2407-03	9.547	0.0	0.013	
K2407-07	0.148	0.0	0.004	
K2407-11	0.180	0.0	0.004	
CCV3	250.726	0.0	0.239	
CCB3	0.307	0.0	0.004	

N	28
Mean	53.846
SD	113.6387
CV%	211.04

Aquakem v. 7.2AQ1

Results from time period:

Mon Apr 15 12:45:50 2019

Mon Apr 15 12:58:42 2019

AS

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.3284	µg/l	4/15/2019 8:02:58	
5.0PPBCN	A	Total CN	P	4.8036	µg/l	4/15/2019 8:02:59	
10PPBCN	A	Total CN	P	10.0187	µg/l	4/15/2019 8:03:00	
50PPBCN	A	Total CN	P	49.2268	µg/l	4/15/2019 8:03:01	
100PPBCN	A	Total CN	P	99.6245	µg/l	4/15/2019 8:03:02	
250PPBCN	A	Total CN	P	251.6878	µg/l	4/15/2019 8:03:03	
500PPBCN	A	Total CN	P	499.3101	µg/l	4/15/2019 8:03:04	
ICV1	S	Total CN	P	94.8236	µg/l	4/15/2019 12:45:50	
ICB1	S	Total CN	P	0.5668	µg/l	4/15/2019 12:45:51	
CCV1	S	Total CN	P	239.4776	µg/l	4/15/2019 12:45:52	
CCB2	S	Total CN	P	0.2542	µg/l	4/15/2019 12:45:53	
PB118886BL	S	Total CN	P	0.2596	µg/l	4/15/2019 12:45:54	
PB118886BS	S	Total CN	P	95.5215	µg/l	4/15/2019 12:45:55	
LOWPB118886	S	Total CN	P	10.0274	µg/l	4/15/2019 12:45:56	
HIGHPB118886	S	Total CN	P	482.1427	µg/l	4/15/2019 12:45:57	
K2199-09	S	Total CN	P	1.2394	µg/l	4/15/2019 12:45:58	
K2199-09DUP	S	Total CN	P	0.4476	µg/l	4/15/2019 12:45:59	
K2199-09MS	S	Total CN	P	34.5235	µg/l	4/15/2019 12:46:00	
K2199-09MSD	S	Total CN	P	34.1033	µg/l	4/15/2019 12:53:22	
K2199-11	S	Total CN	P	1.1416	µg/l	4/15/2019 12:53:23	
K2386-01	S	Total CN	P	1.0049	µg/l	4/15/2019 12:53:24	
CCV2	S	Total CN	P	237.6286	µg/l	4/15/2019 12:53:25	
CCB2	S	Total CN	P	0.2371	µg/l	4/15/2019 12:53:26	
K2390-01	S	Total CN	P	0.4966	µg/l	4/15/2019 12:53:27	
K2390-03	S	Total CN	P	0.6689	µg/l	4/15/2019 12:53:28	
K2390-05	S	Total CN	P	0.5958	µg/l	4/15/2019 12:53:29	
K2397-03	S	Total CN	P	1.6358	µg/l	4/15/2019 12:53:30	
K2397-07	S	Total CN	P	5.3902	µg/l	4/15/2019 12:53:31	
K2397-11	S	Total CN	P	3.0199	µg/l	4/15/2019 12:53:32	
K2397-15	S	Total CN	P	1.5684	µg/l	4/15/2019 12:58:37	
K2407-03	S	Total CN	P	9.5474	µg/l	4/15/2019 12:58:38	
K2407-07	S	Total CN	P	0.1477	µg/l	4/15/2019 12:58:39	
K2407-11	S	Total CN	P	0.1803	µg/l	4/15/2019 12:58:40	
CCV3	S	Total CN	P	250.726	µg/l	4/15/2019 12:58:41	
CCB3	S	Total CN	P	0.3068	µg/l	4/15/2019 12:58:42	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/15/2019 13:04


Test Total CN

Accepted 4/15/2019 8:03

Factor 1068
Bias 0.004

Coeff. of det. 0.999979

Errors

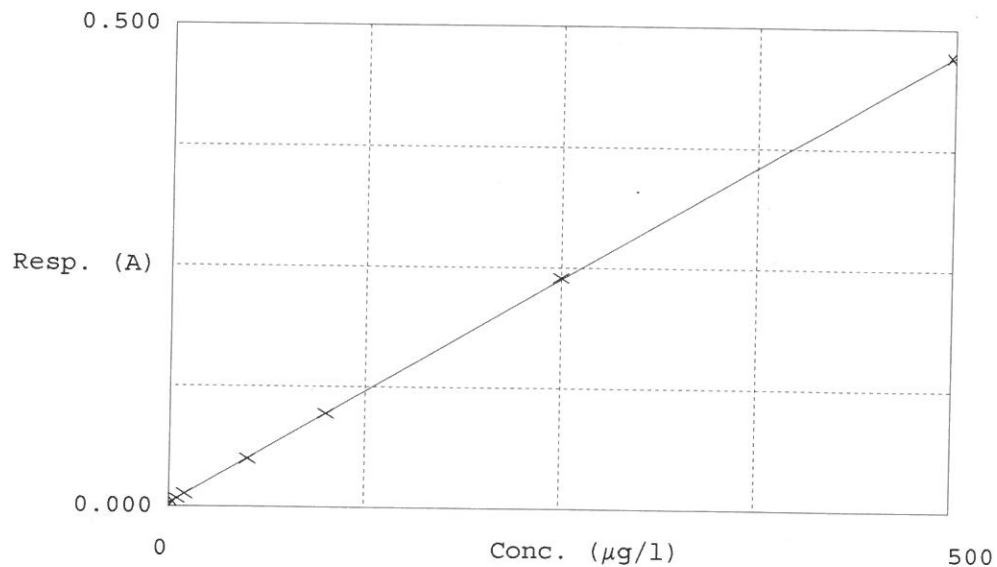

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.3284	0.0000	
2	5.0PPBCN	0.008	4.8036	5.0000	
3	10PPBCN	0.013	10.0187	10.0000	
4	50PPBCN	0.050	49.2268	50.0000	
5	100PPBCN	0.097	99.6245	100.0000	
6	250PPBCN	0.239	251.6878	250.0000	
7	500PPBCN	0.471	499.3101	500.0000	