


LB102115

7470A

INSTRUMENT ID: CU1

Linear ▼

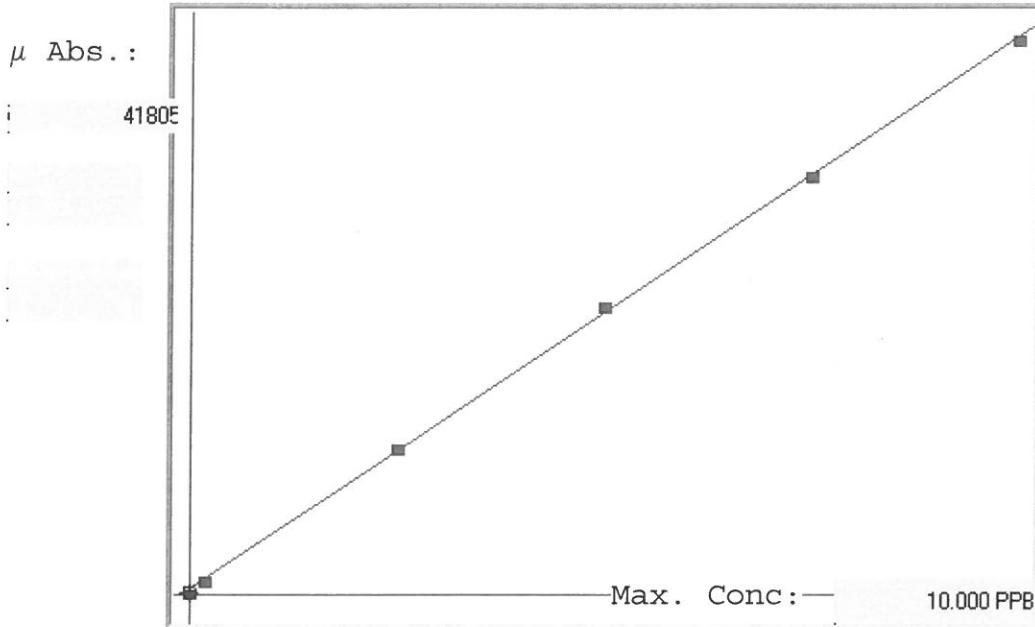

A= 0.0000e+000

B= 2.4004e-004

C= -9.8575e-002

Rho= 0.9998057

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.058	-0.058	168	0.000	168				
0.2	0.200	0.153	-0.047	1047	0.0 %	1047				
2.5	2.500	2.566	0.066	11099	0.0 %	11099				
5.0	5.000	5.130	0.130	21784	0.0 %	21784				
7.5	7.500	7.473	-0.027	31543	0.0 %	31543				
10.0	10.000	9.936	-0.064	41805	0.0 %	41805				

LB102115 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 16 Apr 2019 09:36:35

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	500	168	-	0.0000	7470A	PPB	16 Apr 2019 09:52:53	S	Std
0.2 - 1	502	1047	-	0.2000	7470A	PPB	16 Apr 2019 09:55:01	S	Std
2.5 - 1	525	11099	-	2.5000	7470A	PPB	16 Apr 2019 09:57:09	S	Std
5.0 - 1	550	21784	-	5.0000	7470A	PPB	16 Apr 2019 09:59:17	S	Std
7.5 - 1	575	31543	-	7.5000	7470A	PPB	16 Apr 2019 10:01:24	S	Std
10.0 - 1	5100	41805	-	10.0000	7470A	PPB	16 Apr 2019 10:06:48	S	Std
ICV99 - 1	ICV99	16878	3.9528	-	7470A	PPB	16 Apr 2019 10:09:41	U	SMPL
ICB99 - 1	ICB99	146	-0.0635	-	7470A	PPB	16 Apr 2019 10:11:47	U	SMPL
CCV01 - 1	CCV01	22024	5.1881	-	7470A	PPB	16 Apr 2019 10:13:52	U	SMPL
CCB01 - 1	CCB01	140	-0.0650	-	7470A	PPB	16 Apr 2019 10:15:58	U	SMPL
CRA - 1	CRA	1026	0.1477	-	7470A	PPB	16 Apr 2019 10:18:04	U	SMPL
HighStd - 1	HighStd	42020	9.9880	-	7470A	PPB	16 Apr 2019 10:20:10	U	SMPL
ChkStd - 1	ChkStd	29360	6.9490	-	7470A	PPB	16 Apr 2019 10:22:17	U	SMPL
PB118906BL - 1	PBW	136	-0.0659	-	7470A	PPB	16 Apr 2019 10:24:25	U	SMPL
PB118906BS - 1	LCWSW	18159	4.2603	-	7470A	PPB	16 Apr 2019 10:26:32	U	SMPL
K2199-10 - 1	OR-02-041219-A	226	-0.0443	-	7470A	PPB	16 Apr 2019 10:28:39	U	SMPL
K2199-10DUP - 1	OR-02-041219-ADUP	245	-0.0398	-	7470A	PPB	16 Apr 2019 10:30:47	U	SMPL
K2199-10MS - 1	OR-02-041219-AMS	16911	3.9608	-	7470A	PPB	16 Apr 2019 10:32:55	U	SMPL
K2199-10MSD - 1	OR-02-041219-AMSD	16953	3.9708	-	7470A	PPB	16 Apr 2019 10:35:03	U	SMPL
K2199-12 - 1	OR-02-041219-B	222	-0.0453	-	7470A	PPB	16 Apr 2019 10:37:10	U	SMPL
CCV02 - 1	CCV02	22194	5.2289	-	7470A	PPB	16 Apr 2019 10:39:16	U	SMPL
CCB02 - 1	CCB02	129	-0.0676	-	7470A	PPB	16 Apr 2019 10:41:22	U	SMPL
K2390-02 - 1	3425	264	-0.0352	-	7470A	PPB	16 Apr 2019 10:43:29	U	SMPL
K2390-04 - 1	5124	312	-0.0237	-	7470A	PPB	16 Apr 2019 10:45:35	U	SMPL
K2390-06 - 1	200050	221	-0.0455	-	7470A	PPB	16 Apr 2019 10:47:42	U	SMPL
K2397-04 - 1	TP-1-S	398	-0.0030	-	7470A	PPB	16 Apr 2019 10:49:49	U	SMPL
K2397-08 - 1	TP-1-D	262	-0.0357	-	7470A	PPB	16 Apr 2019 10:51:56	U	SMPL
K2397-12 - 1	TP-3-S	406	-0.0011	-	7470A	PPB	16 Apr 2019 10:54:03	U	SMPL
K2397-16 - 1	TP-3-D	296	-0.0275	-	7470A	PPB	16 Apr 2019 10:56:10	U	SMPL
K2405-03 - 1	B-1D(0-24)	297	-0.0273	-	7470A	PPB	16 Apr 2019 10:58:18	U	SMPL
K2407-04 - 1	TP-11-S	264	-0.0352	-	7470A	PPB	16 Apr 2019 11:00:26	U	SMPL
K2407-08 - 1	TP-11-D	248	-0.0390	-	7470A	PPB	16 Apr 2019 11:02:33	U	SMPL
CCV03 - 1	CCV03	22844	5.3849	-	7470A	PPB	16 Apr 2019 11:04:40	U	SMPL
CCB03 - 1	CCB03	221	-0.0455	-	7470A	PPB	16 Apr 2019 11:06:47	U	SMPL
K2407-12 - 1	TP-17-S	233	-0.0426	-	7470A	PPB	16 Apr 2019 11:08:53	U	SMPL
PB118906TB - 1	PB118866TB	210	-0.0482	-	7470A	PPB	16 Apr 2019 11:11:00	U	SMPL
K2199-10LX5 - 1		170	-0.0578	-	7470A	PPB	16 Apr 2019 11:13:06	U	SMPL
K2199-10A - 1		17371	4.0712	-	7470A	PPB	16 Apr 2019 11:15:13	U	SMPL
CCV04 - 1	CCV04	22190	5.2279	-	7470A	PPB	16 Apr 2019 11:17:19	U	SMPL
CCB04 - 1	CCB04	144	-0.0640	-	7470A	PPB	16 Apr 2019 11:19:27	U	SMPL