

2B102121

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/16/2019 11:57

Test: Total CN

My/h

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.730	0.0	0.092	
ICB1	0.053	0.0	0.005	
CCV1	244.309	0.0	0.225	
CCB1	-0.596	0.0	0.004	
PB118929BL	-0.400	0.0	0.004	
PB118929BS	97.238	0.0	0.092	
LOWPB118929	9.481	0.0	0.013	
HIGHPB118929	484.544	0.0	0.441	
K2423-01	0.320	0.0	0.005	
K2423-01DUP	0.041	0.0	0.005	
K2423-01MS	32.313	0.0	0.034	
K2423-01MSD	32.495	0.0	0.034	
K2423-03	-0.244	0.0	0.004	
K2423-05	-0.111	0.0	0.005	
CCV2	238.787	0.0	0.220	
CCB2	-0.651	0.0	0.004	
K2423-07	-0.474	0.0	0.004	
K2423-09	-0.832	0.0	0.004	
K2423-11	-0.499	0.0	0.004	
K2423-13	-0.349	0.0	0.004	
K2423-15	-0.582	0.0	0.004	
K2423-17	-0.233	0.0	0.004	
K2423-19	-0.372	0.0	0.004	
CCV3	256.174	0.0	0.235	
CCB3	-0.552	0.0	0.004	

N	25
Mean	59.464
SD	120.7134
CV%	203.00

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : AS

Instrument ID : Konelab

4/16/2019 11:17


Test Total CN

Accepted 4/16/2019 11:17

Factor 1111
Bias 0.005

Coeff. of det. 0.999932

Errors

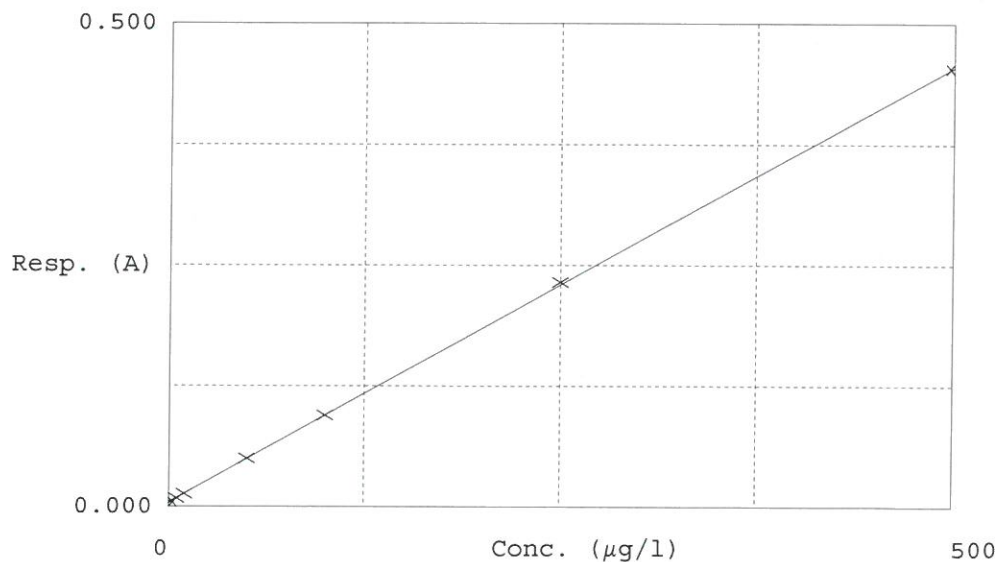

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-1.2071	0.0000	
2	5.0PPBCN	0.009	4.6142	5.0000	
3	10PPBCN	0.013	9.6975	10.0000	
4	50PPBCN	0.050	50.3297	50.0000	
5	100PPBCN	0.095	100.0357	100.0000	
6	250PPBCN	0.233	253.1204	250.0000	
7	500PPBCN	0.453	498.4096	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Tue Apr 16 10:41:37 2019

Tue Apr 16 11:56:48 2019

✓AS

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-1.2071	µg/l	4/16/2019 11:17:12	
5.OPPBCN	A	Total CN	P	4.6142	µg/l	4/16/2019 11:17:13	
10PPBCN	A	Total CN	P	9.6975	µg/l	4/16/2019 11:17:14	
50PPBCN	A	Total CN	P	50.3297	µg/l	4/16/2019 11:17:15	
100PPBCN	A	Total CN	P	100.0357	µg/l	4/16/2019 11:17:16	
250PPBCN	A	Total CN	P	253.1204	µg/l	4/16/2019 11:17:17	
500PPBCN	A	Total CN	P	498.4096	µg/l	4/16/2019 11:17:18	
ICV1	S	Total CN	P	96.7305	µg/l	4/16/2019 11:45:20	
ICB1	S	Total CN	P	0.0528	µg/l	4/16/2019 11:45:21	
CCV1	S	Total CN	P	244.3089	µg/l	4/16/2019 11:45:22	
CCB1	S	Total CN	P	-0.5958	µg/l	4/16/2019 11:45:23	
PB118929BL	S	Total CN	P	-0.4	µg/l	4/16/2019 11:45:24	
PB118929BS	S	Total CN	P	97.2383	µg/l	4/16/2019 11:45:25	
LOWPB118929	S	Total CN	P	9.4814	µg/l	4/16/2019 11:45:26	
HIGHPB118929	S	Total CN	P	484.5443	µg/l	4/16/2019 11:45:27	
K2423-01	S	Total CN	P	0.32	µg/l	4/16/2019 11:45:28	
K2423-01DUP	S	Total CN	P	0.0406	µg/l	4/16/2019 11:45:29	
K2423-01MS	S	Total CN	P	32.313	µg/l	4/16/2019 11:45:30	
K2423-01MSD	S	Total CN	P	32.4952	µg/l	4/16/2019 11:52:55	
K2423-03	S	Total CN	P	-0.2443	µg/l	4/16/2019 11:52:56	
K2423-05	S	Total CN	P	-0.1105	µg/l	4/16/2019 11:52:57	
CCV2	S	Total CN	P	238.7871	µg/l	4/16/2019 11:52:58	
CCB2	S	Total CN	P	-0.6512	µg/l	4/16/2019 11:52:59	
K2423-07	S	Total CN	P	-0.474	µg/l	4/16/2019 11:53:00	
K2423-09	S	Total CN	P	-0.8317	µg/l	4/16/2019 11:53:01	
K2423-11	S	Total CN	P	-0.4988	µg/l	4/16/2019 11:53:02	
K2423-13	S	Total CN	P	-0.3486	µg/l	4/16/2019 11:53:03	
K2423-15	S	Total CN	P	-0.5822	µg/l	4/16/2019 11:53:04	
K2423-17	S	Total CN	P	-0.2326	µg/l	4/16/2019 11:53:05	
K2423-19	S	Total CN	P	-0.3719	µg/l	4/16/2019 11:56:46	
CCV3	S	Total CN	P	256.1744	µg/l	4/16/2019 11:56:47	
CCB3	S	Total CN	P	-0.5523	µg/l	4/16/2019 11:56:48	