

2B102164

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/17/2019 15:46

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	100.240	0.0	0.091	
ICB1	-0.438	0.0	0.005	
CCV1	236.926	0.0	0.209	
CCB1	-0.900	0.0	0.004	
PB118987BL	-0.782	0.0	0.004	
PB118987BS	101.933	0.0	0.093	
K2437-01	-0.622	0.0	0.005	
K2437-01DUP	-0.514	0.0	0.005	
K2437-01MS	31.126	0.0	0.032	
K2437-01MSD	31.270	0.0	0.032	
K2441-03	-0.214	0.0	0.005	
K2442-03	-0.998	0.0	0.004	
K2442-07	-0.875	0.0	0.004	
K2442-11	-0.354	0.0	0.005	
CCV2	237.853	0.0	0.210	
CCB2	-0.777	0.0	0.004	
K2442-15	-0.597	0.0	0.005	
K2444-01	0.296	0.0	0.005	
K2444-03	0.416	0.0	0.005	
K2453-01	6.577	0.0	0.011	
CCV3	236.585	0.0	0.209	
CCB3	-0.764	0.0	0.004	

N	22
Mean	44.336
SD	83.9132
CV%	189.27

Aquakem v. 7.2AQ1

Results from time period:

Wed Apr 17 15:31:54 2019

Wed Apr 17 15:39:39 2019

AS

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-1.4165	µg/l	4/17/2019 12:38:59	
5.0PPBCN	A	Total CN	P	4.0122	µg/l	4/17/2019 12:39:00	
10PPBCN	A	Total CN	P	9.3458	µg/l	4/17/2019 12:39:01	
50PPBCN	A	Total CN	P	51.3101	µg/l	4/17/2019 12:39:02	
100PPBCN	A	Total CN	P	105.9141	µg/l	4/17/2019 12:39:03	
250PPBCN	A	Total CN	P	244.2505	µg/l	4/17/2019 12:39:04	
500PPBCN	A	Total CN	P	501.5839	µg/l	4/17/2019 12:39:05	
ICV1	S	Total CN	P	100.2398	µg/l	4/17/2019 15:31:54	
ICB1	S	Total CN	P	-0.4384	µg/l	4/17/2019 15:31:55	
CCV1	S	Total CN	P	236.9256	µg/l	4/17/2019 15:31:56	
CCB1	S	Total CN	P	-0.8999	µg/l	4/17/2019 15:31:57	
PB118987BL	S	Total CN	P	-0.7817	µg/l	4/17/2019 15:31:58	
PB118987BS	S	Total CN	P	101.9328	µg/l	4/17/2019 15:31:59	
K2437-01	S	Total CN	P	-0.6217	µg/l	4/17/2019 15:32:00	
K2437-01DUP	S	Total CN	P	-0.5136	µg/l	4/17/2019 15:32:01	
K2437-01MS	S	Total CN	P	31.1258	µg/l	4/17/2019 15:32:02	
K2437-01MSD	S	Total CN	P	31.2704	µg/l	4/17/2019 15:32:03	
K2441-03	S	Total CN	P	-0.2136	µg/l	4/17/2019 15:32:04	
K2442-03	S	Total CN	P	-0.9985	µg/l	4/17/2019 15:39:29	
K2442-07	S	Total CN	P	-0.8751	µg/l	4/17/2019 15:39:30	
K2442-11	S	Total CN	P	-0.3536	µg/l	4/17/2019 15:39:31	
CCV2	S	Total CN	P	237.8533	µg/l	4/17/2019 15:39:32	
CCB2	S	Total CN	P	-0.7766	µg/l	4/17/2019 15:39:33	
K2442-15	S	Total CN	P	-0.5966	µg/l	4/17/2019 15:39:34	
K2444-01	S	Total CN	P	0.2956	µg/l	4/17/2019 15:39:35	
K2444-03	S	Total CN	P	0.4162	µg/l	4/17/2019 15:39:36	
K2453-01	S	Total CN	P	6.5768	µg/l	4/17/2019 15:39:37	
CCV3	S	Total CN	P	236.5848	µg/l	4/17/2019 15:39:38	
CCB3	S	Total CN	P	-0.7641	µg/l	4/17/2019 15:39:39	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AB

Instrument ID : Konelab

4/17/2019 12:39


Test Total CN

Accepted 4/17/2019 12:39

Factor 1161
Bias 0.005

Coeff. of det. 0.999632

Errors

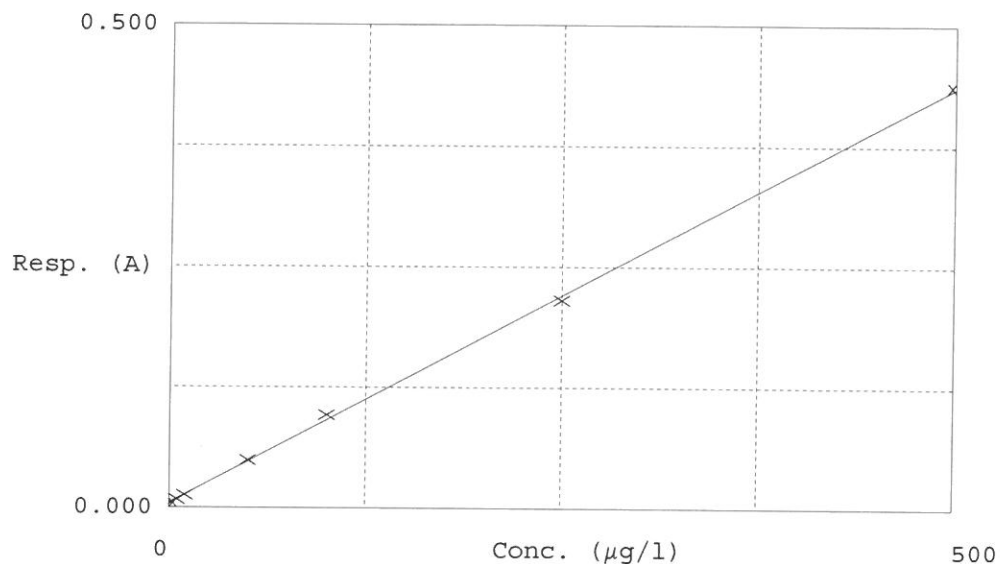

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-1.4165	0.0000	
2	5.0PPBCN	0.009	4.0122	5.0000	
3	10PPBCN	0.013	9.3458	10.0000	
4	50PPBCN	0.049	51.3101	50.0000	
5	100PPBCN	0.096	105.9141	100.0000	
6	250PPBCN	0.215	244.2505	250.0000	
7	500PPBCN	0.437	501.5839	500.0000	