


LB102286

7471B

INSTRUMENT ID : CV1

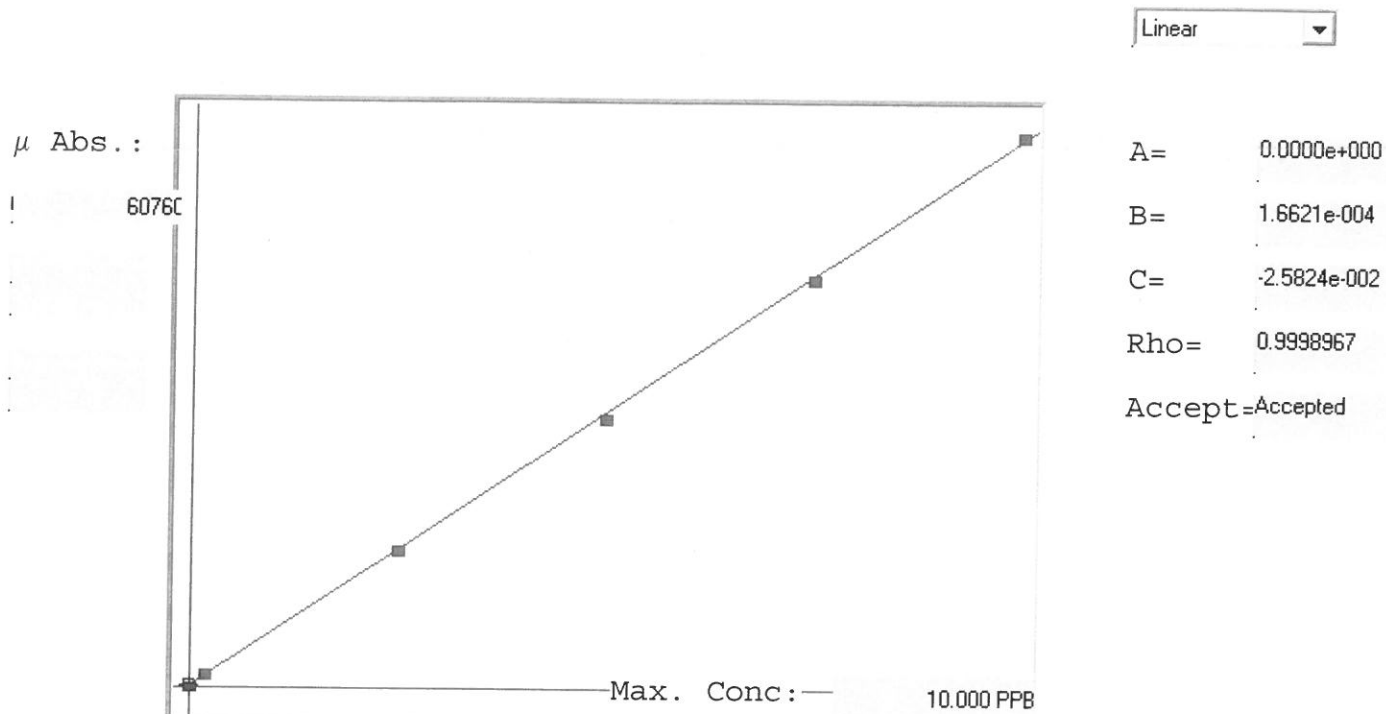

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.026	0.026	309	0.000	309				
0.2	0.200	0.232	0.032	1551	0.0 %	1551				
2.5	2.500	2.500	0.000	15200	0.0 %	15200				
5.0	5.000	4.909	-0.091	29689	0.0 %	29689				
7.5	7.500	7.461	-0.039	45043	0.0 %	45043				
10.0	10.000	10.073	0.073	60760	0.0 %	60760				

LB102286 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 23 Apr 2019 08:16:02

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50-0	309	-	0.00007471B	PPB	23 Apr 2019 08:21:59	S	Std
0.2 - 1	50-2	1551	-	0.20007471B	PPB	23 Apr 2019 08:24:17	S	Std
2.5 - 1	52-5	15200	-	2.50007471B	PPB	23 Apr 2019 08:26:34	S	Std
5.0 - 1	55-0	29689	-	5.00007471B	PPB	23 Apr 2019 08:28:51	S	Std
7.5 - 1	57-5	45043	-	7.50007471B	PPB	23 Apr 2019 08:31:08	S	Std
10.0 - 1	510-0	60760	-	10.00007471B	PPB	23 Apr 2019 08:33:24	S	Std
ICV15 - 1	ICV15	24242	4.0033	-7471B	PPB	23 Apr 2019 08:37:22	U	SMPL
ICB15 - 1	ICB15	236	0.0134	-7471B	PPB	23 Apr 2019 08:39:37	U	SMPL
CCV75 - 1	CCV75	30482	5.0404	-7471B	PPB	23 Apr 2019 08:41:52	U	SMPL
CCB75 - 1	CCB75	235	0.0132	-7471B	PPB	23 Apr 2019 08:44:08	U	SMPL
CRA - 1	CRA	1587	0.2379	-7471B	PPB	23 Apr 2019 08:46:22	U	SMPL
HighStd - 1	HighStd	60308	9.9977	-7471B	PPB	23 Apr 2019 08:48:38	U	SMPL
ChkStd - 1	ChkStd	42045	6.9623	-7471B	PPB	23 Apr 2019 08:50:54	U	SMPL
PB119124BL - 1	PBS	54	-0.0168	-7471B	PPB	23 Apr 2019 08:53:11	U	SMPL
PB119124BS - 1	LCSS	21109	3.4826	-7471B	PPB	23 Apr 2019 08:55:29	U	SMPL
K2204-03 - 1	TR-05-042219	1448	0.2148	-7471B	PPB	23 Apr 2019 08:57:46	U	SMPL
K2464-01 - 1	M-COMP-4.18.19	23166	3.8245	-7471B	PPB	23 Apr 2019 09:00:02	U	SMPL
K2464-01DUP - 1	M-COMP-4.18.19DUP	23128	3.8182	-7471B	PPB	23 Apr 2019 09:02:19	U	SMPL
K2464-01MS - 1	M-COMP-4.18.19MS	47862	7.9291	-7471B	PPB	23 Apr 2019 09:04:37	U	SMPL
K2464-01MSD - 1	M-COMP-4.18.19MSD	47617	7.8884	-7471B	PPB	23 Apr 2019 09:06:53	U	SMPL
CCV76 - 1	CCV76	30538	5.0498	-7471B	PPB	23 Apr 2019 09:09:11	U	SMPL
CCB76 - 1	CCB76	279	0.0205	-7471B	PPB	23 Apr 2019 09:11:27	U	SMPL
K2465-01 - 1	Q-COMP-4.18.19	684	0.0879	-7471B	PPB	23 Apr 2019 09:13:44	U	SMPL
K2510-01 - 1	SOIL-PILE-A	1741	0.2635	-7471B	PPB	23 Apr 2019 09:15:59	U	SMPL
K2510-03 - 1	SOIL-PILE-B	1660	0.2501	-7471B	PPB	23 Apr 2019 09:18:15	U	SMPL
K2514-01 - 1	FK-EF-01-007-ABCD	2927	0.4607	-7471B	PPB	23 Apr 2019 09:20:31	U	SMPL
K2515-03 - 1	TP-15	674	0.0862	-7471B	PPB	23 Apr 2019 09:22:47	U	SMPL
K2515-07 - 1	TP-10	488	0.0553	-7471B	PPB	23 Apr 2019 09:25:04	U	SMPL
K2515-11 - 1	TP-9	1942	0.2969	-7471B	PPB	23 Apr 2019 09:27:21	U	SMPL
K2515-15 - 1	TP-12	1001	0.1405	-7471B	PPB	23 Apr 2019 09:29:38	U	SMPL
K2515-19 - 1	TP-13	2724	0.4269	-7471B	PPB	23 Apr 2019 09:31:54	U	SMPL
K2515-23 - 1	TP-16	1874	0.2856	-7471B	PPB	23 Apr 2019 09:34:10	U	SMPL
CCV77 - 1	CCV77	31349	5.1845	-7471B	PPB	23 Apr 2019 09:36:26	U	SMPL
CCB77 - 1	CCB77	238	0.0137	-7471B	PPB	23 Apr 2019 09:38:42	U	SMPL
K2518-02 - 1	MUDDY-BAGS	5035	0.8110	-7471B	PPB	23 Apr 2019 09:40:58	U	SMPL
K2518-05 - 1	MUDDY-SOIL	4687	0.7532	-7471B	PPB	23 Apr 2019 09:43:13	U	SMPL
K2522-07 - 1	SP-WOODBURY	4035	0.6448	-7471B	PPB	23 Apr 2019 09:45:29	U	SMPL
K2526-01 - 1	SOIL-ROLLOFFS	5052	0.8138	-7471B	PPB	23 Apr 2019 09:47:45	U	SMPL
K2528-01 - 1	S042219	5365	0.8659	-7471B	PPB	23 Apr 2019 09:50:00	U	SMPL
K2529-01 - 1	P3P4042219	917	0.1266	-7471B	PPB	23 Apr 2019 09:52:17	U	SMPL
PB119130BL - 1	PBS	215	0.0099	-7471B	PPB	23 Apr 2019 09:54:34	U	SMPL
PB119130BS - 1	LCSS	21706	3.5818	-7471B	PPB	23 Apr 2019 09:56:51	U	SMPL
K2532-03 - 1	TP-5	2934	0.4618	-7471B	PPB	23 Apr 2019 09:59:08	U	SMPL
K2532-07 - 1	TP-2	3817	0.6086	-7471B	PPB	23 Apr 2019 10:01:24	U	SMPL
CCV78 - 1	CCV78	32547	5.3837	-7471B	PPB	23 Apr 2019 10:03:40	U	SMPL
CCB78 - 1	CCB78	147	-0.0014	-7471B	PPB	23 Apr 2019 10:05:56	U	SMPL
K2532-11 - 1	TP-3	1720	0.2600	-7471B	PPB	23 Apr 2019 10:08:12	U	SMPL
K2532-15 - 1	TP-17	4849	0.7801	-7471B	PPB	23 Apr 2019 10:10:28	U	SMPL
K2532-19 - 1	TP-14	2171	0.3350	-7471B	PPB	23 Apr 2019 10:12:44	U	SMPL
K2532-23 - 1	TP-4	3250	0.5143	-7471B	PPB	23 Apr 2019 10:14:59	U	SMPL
K2532-23DUP - 1	TP-4DUP	3264	0.5167	-7471B	PPB	23 Apr 2019 10:17:15	U	SMPL
K2532-23MS - 1	TP-4MS	26481	4.3755	-7471B	PPB	23 Apr 2019 10:19:32	U	SMPL
K2532-23MSD - 1	TP-4MSD	26283	4.3425	-7471B	PPB	23 Apr 2019 10:21:49	U	SMPL
K2464-01LX5 - 1		4776	0.7680	-7471B	PPB	23 Apr 2019 10:24:07	U	SMPL
K2464-01A - 1		47543	7.8761	-7471B	PPB	23 Apr 2019 10:26:24	U	SMPL
K2532-23LX5 - 1		709	0.0920	-7471B	PPB	23 Apr 2019 10:28:40	U	SMPL
CCV79 - 1	CCV79	32716	5.4117	-7471B	PPB	23 Apr 2019 10:30:57	U	SMPL
CCB79 - 1	CCB79	267	0.0186	-7471B	PPB	23 Apr 2019 10:33:13	U	SMPL
K2532-23A - 1		26394	4.3610	-7471B	PPB	23 Apr 2019 10:35:29	U	SMPL
CCV80 - 1	CCV80	31983	5.2899	-7471B	PPB	23 Apr 2019 10:37:45	U	SMPL
CCB80 - 1	CCB80	38	-0.0195	-7471B	PPB	23 Apr 2019 10:40:01	U	SMPL