


LB102318

7470A

INSTRUMENT ID: CV1

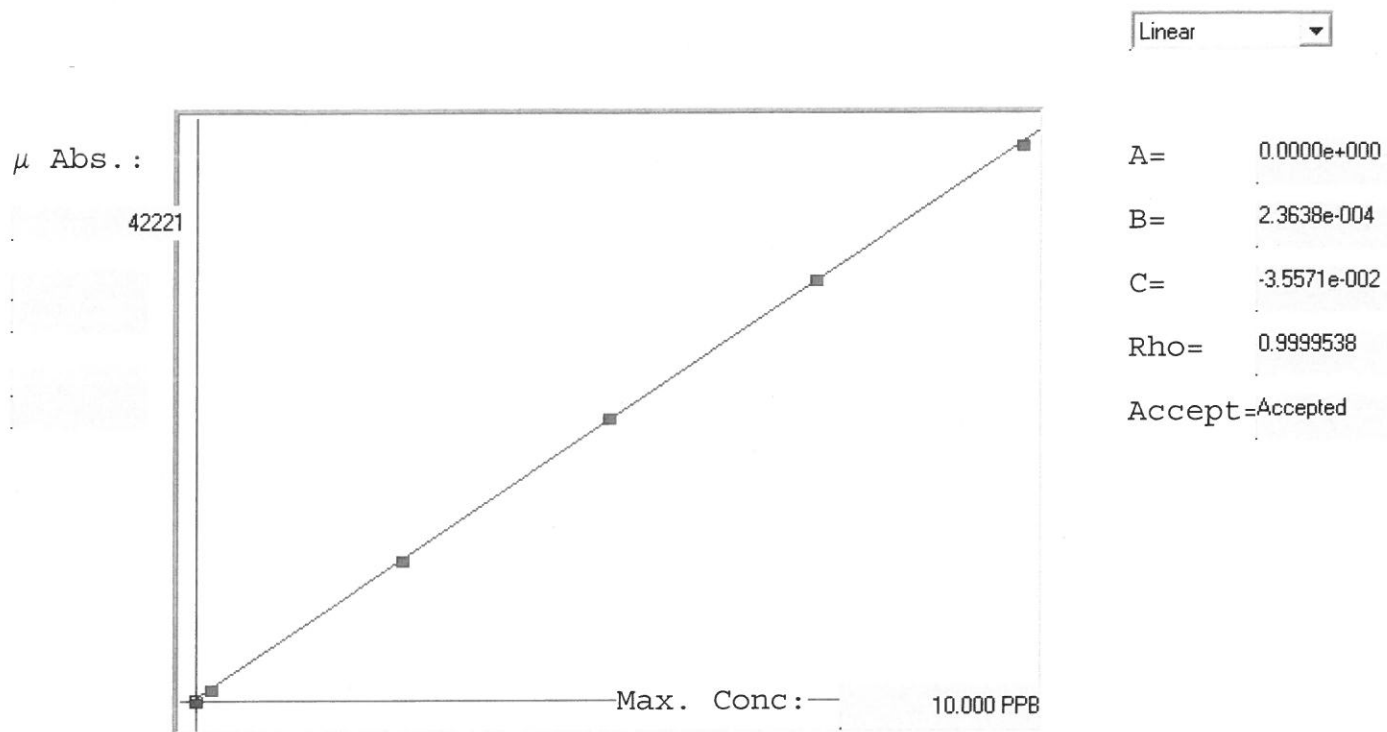

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.015	-0.015	85	0.000	85				
0.2	0.200	0.180	-0.020	911	0.0 %	911				
2.5	2.500	2.503	0.003	10741	0.0 %	10741				
5.0	5.000	5.046	0.046	21499	0.0 %	21499				
7.5	7.500	7.541	0.041	32052	0.0 %	32052				
10.0	10.000	9.945	-0.055	42221	0.0 %	42221				

LB102318 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 24 Apr 2019 10:18:08

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	85	-	0.0000	7470A	PPB	24 Apr 2019 10:35:54	S	Std
0.2 - 1	50.2	911	-	0.2000	7470A	PPB	24 Apr 2019 10:38:02	S	Std
2.5 - 1	52.5	10741	-	2.5000	7470A	PPB	24 Apr 2019 10:40:10	S	Std
5.0 - 1	55.0	21499	-	5.0000	7470A	PPB	24 Apr 2019 10:42:18	S	Std
7.5 - 1	57.5	32052	-	7.5000	7470A	PPB	24 Apr 2019 10:44:26	S	Std
10.0 - 1	510.0	42221	-	10.0000	7470A	PPB	24 Apr 2019 10:46:33	S	Std
ICV18 - 1	ICV18	16609	3.8905	-	7470A	PPB	24 Apr 2019 10:49:29	U	SMPL
ICB18 - 1	ICB18	95	-0.0131	-	7470A	PPB	24 Apr 2019 10:51:35	U	SMPL
CCV85 - 1	CCV85	21304	5.0004	-	7470A	PPB	24 Apr 2019 10:53:41	U	SMPL
CCB85 - 1	CCB85	58	-0.0219	-	7470A	PPB	24 Apr 2019 10:55:47	U	SMPL
CRA - 1	CRA	922	0.1824	-	7470A	PPB	24 Apr 2019 10:57:53	U	SMPL
HighStd - 1	HighStd	42130	9.9233	-	7470A	PPB	24 Apr 2019 10:59:58	U	SMPL
ChkStd - 1	ChkStd	30106	7.0810	-	7470A	PPB	24 Apr 2019 11:02:05	U	SMPL
PB119178BL - 1	PBW	38	-0.0266	-	7470A	PPB	24 Apr 2019 11:04:12	U	SMPL
PB119178BS - 1	LCSW	16569	3.8811	-	7470A	PPB	24 Apr 2019 11:06:18	U	SMPL
K2204-04 - 1	TR-05-042219	85	-0.0155	-	7470A	PPB	24 Apr 2019 11:08:26	U	SMPL
K2204-04DUP - 1	TR-05-042219DUP	128	-0.0053	-	7470A	PPB	24 Apr 2019 11:10:36	U	SMPL
K2204-04MS - 1	TR-05-042219MS	17562	4.1158	-	7470A	PPB	24 Apr 2019 11:12:45	U	SMPL
K2204-04MSD - 1	TR-05-042219MSD	17321	4.0588	-	7470A	PPB	24 Apr 2019 11:14:54	U	SMPL
K2518-04 - 1	MUDDY-BAGS	146	-0.0011	-	7470A	PPB	24 Apr 2019 11:17:00	U	SMPL
CCV86 - 1	CCV86	21430	5.0301	-	7470A	PPB	24 Apr 2019 11:19:06	U	SMPL
CCB86 - 1	CCB86	82	-0.0162	-	7470A	PPB	24 Apr 2019 11:21:12	U	SMPL
K2518-07 - 1	MUDDY-SOIL	167	0.0039	-	7470A	PPB	24 Apr 2019 11:23:18	U	SMPL
K2522-08 - 1	SP-WOODBURY	190	0.0093	-	7470A	PPB	24 Apr 2019 11:25:24	U	SMPL
K2526-03 - 1	SOIL-ROLLOFFS	152	0.0004	-	7470A	PPB	24 Apr 2019 11:27:30	U	SMPL
K2532-04 - 1	TP-5	141	-0.0022	-	7470A	PPB	24 Apr 2019 11:29:37	U	SMPL
K2532-08 - 1	TP-2	150	-0.0001	-	7470A	PPB	24 Apr 2019 11:31:44	U	SMPL
K2532-12 - 1	TP-3	126	-0.0058	-	7470A	PPB	24 Apr 2019 11:33:51	U	SMPL
K2532-16 - 1	TP-17	588	0.1034	-	7470A	PPB	24 Apr 2019 11:35:58	U	SMPL
K2532-20 - 1	TP-14	237	0.0205	-	7470A	PPB	24 Apr 2019 11:38:06	U	SMPL
K2532-24 - 1	TP-4	151	0.0001	-	7470A	PPB	24 Apr 2019 11:40:14	U	SMPL
PB119179BL - 1	PBW	82	-0.0162	-	7470A	PPB	24 Apr 2019 11:42:21	U	SMPL
CCV87 - 1	CCV87	21792	5.1157	-	7470A	PPB	24 Apr 2019 11:44:27	U	SMPL
CCB87 - 1	CCB87	56	-0.0223	-	7470A	PPB	24 Apr 2019 11:46:34	U	SMPL
PB119179BS - 1	LCSW	16491	3.8626	-	7470A	PPB	24 Apr 2019 11:48:40	U	SMPL
K2522-02 - 1	WELL-1	123	-0.0065	-	7470A	PPB	24 Apr 2019 11:50:47	U	SMPL
K2522-02DUP - 1	WELL-1DUP	142	-0.0020	-	7470A	PPB	24 Apr 2019 11:52:53	U	SMPL
K2522-02MS - 1	WELL-1MS	16548	3.8761	-	7470A	PPB	24 Apr 2019 11:55:00	U	SMPL
K2522-02MSD - 1	WELL-1MSD	16720	3.9168	-	7470A	PPB	24 Apr 2019 11:57:07	U	SMPL
K2522-05 - 1	WELL-2	113	-0.0089	-	7470A	PPB	24 Apr 2019 11:59:15	U	SMPL
PB119180BL - 1	PBW	103	-0.0112	-	7470A	PPB	24 Apr 2019 12:01:22	U	SMPL
PB119180BS - 1	LCSW	16968	3.9754	-	7470A	PPB	24 Apr 2019 12:03:30	U	SMPL
K2522-01 - 1	WELL-1	7537	1.7461	-	7470A	PPB	24 Apr 2019 12:05:37	U	SMPL
K2522-01DUP - 1	WELL-1DUP	7476	1.7316	-	7470A	PPB	24 Apr 2019 12:07:44	U	SMPL
CCV88 - 1	CCV88	22970	5.3942	-	7470A	PPB	24 Apr 2019 12:09:50	U	SMPL
CCB88 - 1	CCB88	52	-0.0233	-	7470A	PPB	24 Apr 2019 12:11:57	U	SMPL
K2522-01MS - 1	WELL-1MS	22364	5.2509	-	7470A	PPB	24 Apr 2019 12:19:57	U	SMPL
K2522-01MSD - 1	WELL-1MSD	23240	5.4580	-	7470A	PPB	24 Apr 2019 12:22:03	U	SMPL
K2522-04 - 1	WELL-2	11268	2.6280	-	7470A	PPB	24 Apr 2019 12:24:09	U	SMPL
PB119178TB - 1	PB119125TB	98	-0.0124	-	7470A	PPB	24 Apr 2019 12:26:17	U	SMPL
PB119179TB - 1	PB119128TB	126	-0.0058	-	7470A	PPB	24 Apr 2019 12:28:25	U	SMPL
K2204-04LX5 - 1		98	-0.0124	-	7470A	PPB	24 Apr 2019 12:30:33	U	SMPL
K2204-04A - 1		17333	4.0617	-	7470A	PPB	24 Apr 2019 12:32:40	U	SMPL
K2522-02LX5 - 1		62	-0.0209	-	7470A	PPB	24 Apr 2019 12:34:48	U	SMPL
K2522-02A - 1		16474	3.8586	-	7470A	PPB	24 Apr 2019 12:36:57	U	SMPL
K2522-01LX5 - 1		1301	0.2720	-	7470A	PPB	24 Apr 2019 12:39:04	U	SMPL
CCV89 - 1	CCV89	19817	4.6489	-	7470A	PPB	24 Apr 2019 12:41:11	U	SMPL
CCB89 - 1	CCB89	-1	-0.0358	-	7470A	PPB	24 Apr 2019 12:43:17	U	SMPL
K2522-01A - 1		24243	5.6951	-	7470A	PPB	24 Apr 2019 12:45:24	U	SMPL
CCV90 - 1	CCV90	20592	4.8321	-	7470A	PPB	24 Apr 2019 12:50:21	U	SMPL
CCB90 - 1	CCB90	37	-0.0268	-	7470A	PPB	24 Apr 2019 12:52:28	U	SMPL