

LB102326

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/24/2019 15:14

Test: Routine
Total CN

ug/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	98.536	0.0	0.096	
ICB1	0.646	0.0	0.005	
AS CCV1 CCV2	246.127	0.0	0.233	
CCB1 CCB2	-0.024	0.0	0.004	
K2200-12	0.268	0.0	0.004	
K2541-02	0.149	0.0	0.004	
K2542-04	0.120	0.0	0.004	
K2542-08	0.217	0.0	0.004	
K2542-12	0.141	0.0	0.004	
K2475-04	0.186	0.0	0.004	
K2475-06	0.035	0.0	0.004	
K2475-08	0.184	0.0	0.004	
K2518-04	0.208	0.0	0.004	
AS CCV2 CCV3	242.487	0.0	0.230	
CCB2 CCB3	-0.091	0.0	0.004	
K2518-07	-0.004	0.0	0.004	
K2522-08	0.087	0.0	0.004	
K2526-03	0.015	0.0	0.004	
K2528-01	0.136	0.0	0.004	
K2529-05	-0.154	0.0	0.004	
K2532-04	0.004	0.0	0.004	
K2532-08	-0.231	0.0	0.004	
K2532-12	-0.165	0.0	0.004	
K2532-16	0.059	0.0	0.004	
K2532-20	0.099	0.0	0.004	
AS CCV3 CCV4	244.069	0.0	0.231	
CCB3 CCB4	0.122	0.0	0.004	
K2532-24	-0.176	0.0	0.004	
PB119155BL	0.014	0.0	0.004	
K2522-02	0.274	0.0	0.004	
K2522-02DUP	0.029	0.0	0.004	
K2522-05	0.393	0.0	0.004	
AS CCV4 CCV5	244.212	0.0	0.231	
CCB4 CCB5	0.430	0.0	0.004	
PB119184BL	0.038	0.0	0.004	
K2200-08	0.178	0.0	0.004	
K2200-08DUP	0.083	0.0	0.004	
K2200-10	0.233	0.0	0.004	
K2542-16	0.131	0.0	0.004	
K2542-20	0.212	0.0	0.004	
PB119154BL	0.059	0.0	0.004	
K2204-04	0.134	0.0	0.004	
K2204-04DUP	0.243	0.0	0.004	
K2475-02	0.108	0.0	0.004	
CCV5	237.390	0.0	0.225	
CCB5	-0.200	0.0	0.004	

=====
Test results

Aquakem 7.2AQ1

Page: 2

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/24/2019 15:14

Test: ^{Deactive}
~~Total~~ CN

Sample Id Result Dil. 1 + Response Ô□,,

N	46
Mean	28.631
SD	77.0203
CV%	269.01

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

4/24/2019 12:03

Reviewed by : AS

Instrument ID : Konelab


Test Total CN

Accepted 4/24/2019 12:03

Factor 1074
Bias 0.004

Coeff. of det. 0.999969

Errors

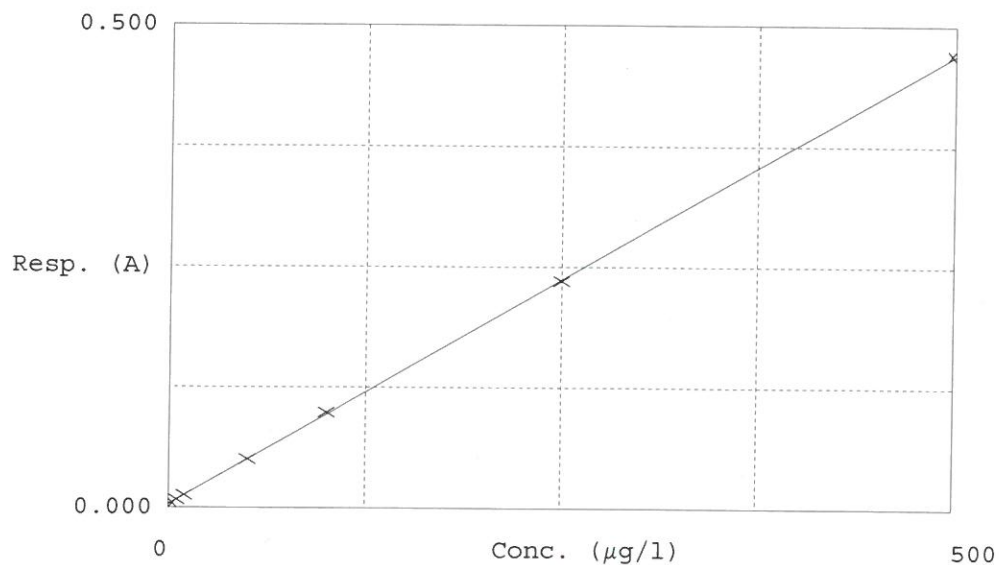

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.2010	0.0000	
2	5.0PPBCN	0.008	4.8136	5.0000	
3	10PPBCN	0.013	9.6697	10.0000	
4	50PPBCN	0.050	49.9230	50.0000	
5	100PPBCN	0.099	101.9363	100.0000	
6	250PPBCN	0.235	248.4589	250.0000	
7	500PPBCN	0.470	500.3994	500.0000	

AS

Aquakem v. 7.2AQ1

Results from time period:

Wed Apr 24 14:15:13 2019

Wed Apr 24 15:10:36 2019

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.201	µg/l	4/24/2019 12:02:45	
5.OPPBCN	A	Reactive CN	P	4.8136	µg/l	4/24/2019 12:02:46	
10PPBCN	A	Reactive CN	P	9.6697	µg/l	4/24/2019 12:02:47	
50PPBCN	A	Reactive CN	P	49.923	µg/l	4/24/2019 12:02:48	
100PPBCN	A	Reactive CN	P	101.9363	µg/l	4/24/2019 12:02:49	
250PPBCN	A	Reactive CN	P	248.4589	µg/l	4/24/2019 12:02:50	
500PPBCN	A	Reactive CN	P	500.3994	µg/l	4/24/2019 12:02:51	
ICV1	S	Reactive CN	P	98.5359	µg/l	4/24/2019 14:15:13	
ICB1	S	Reactive CN	P	0.6457	µg/l	4/24/2019 14:15:14	
CCV1	S	Reactive CN	P	246.1271	µg/l	4/24/2019 14:15:16	
CCB1	S	Reactive CN	P	-0.0239	µg/l	4/24/2019 14:15:17	
K2200-12	S	Reactive CN	P	0.2677	µg/l	4/24/2019 14:27:37	
K2541-02	S	Reactive CN	P	0.1487	µg/l	4/24/2019 14:27:38	
K2542-04	S	Reactive CN	P	0.1204	µg/l	4/24/2019 14:27:39	
K2542-08	S	Reactive CN	P	0.2167	µg/l	4/24/2019 14:27:40	
K2542-12	S	Reactive CN	P	0.1407	µg/l	4/24/2019 14:27:41	
K2475-04	S	Reactive CN	P	0.1857	µg/l	4/24/2019 14:27:42	
K2475-06	S	Reactive CN	P	0.0352	µg/l	4/24/2019 14:27:43	
K2475-08	S	Reactive CN	P	0.1838	µg/l	4/24/2019 14:27:44	
K2518-04	S	Reactive CN	P	0.2084	µg/l	4/24/2019 14:27:45	
CCV2	S	Reactive CN	P	242.4869	µg/l	4/24/2019 14:27:46	
CCB2	S	Reactive CN	P	-0.0909	µg/l	4/24/2019 14:35:08	
K2518-07	S	Reactive CN	P	-0.0044	µg/l	4/24/2019 14:35:09	
K2522-08	S	Reactive CN	P	0.0869	µg/l	4/24/2019 14:35:10	
K2526-03	S	Reactive CN	P	0.0151	µg/l	4/24/2019 14:35:11	
K2528-01	S	Reactive CN	P	0.1357	µg/l	4/24/2019 14:35:12	
K2529-05	S	Reactive CN	P	-0.1544	µg/l	4/24/2019 14:35:13	
K2532-04	S	Reactive CN	P	0.0044	µg/l	4/24/2019 14:35:14	
K2532-08	S	Reactive CN	P	-0.2313	µg/l	4/24/2019 14:35:15	
K2532-12	S	Reactive CN	P	-0.1651	µg/l	4/24/2019 14:35:16	
K2532-16	S	Reactive CN	P	0.0592	µg/l	4/24/2019 14:35:17	
K2532-20	S	Reactive CN	P	0.0987	µg/l	4/24/2019 14:35:18	
CCV3	S	Reactive CN	P	244.0687	µg/l	4/24/2019 14:42:43	
CCB3	S	Reactive CN	P	0.122	µg/l	4/24/2019 14:42:44	
K2532-24	S	Reactive CN	P	-0.1764	µg/l	4/24/2019 14:42:45	
PB119155BL	S	Reactive CN	P	0.0142	µg/l	4/24/2019 14:42:46	
K2522-02	S	Reactive CN	P	0.2736	µg/l	4/24/2019 14:42:47	
K2522-02DUP	S	Reactive CN	P	0.0291	µg/l	4/24/2019 14:42:48	
K2522-05	S	Reactive CN	P	0.3932	µg/l	4/24/2019 14:42:49	
CCV4	S	Reactive CN	P	244.212	µg/l	4/24/2019 14:42:52	
CCB4	S	Reactive CN	P	0.4302	µg/l	4/24/2019 14:42:53	
PB119184BL	S	Reactive CN	P	0.0378	µg/l	4/24/2019 15:07:48	

AS

K2200-08	S	Reactive CN	P	0.1779 µg/l	4/24/2019 15:07:49
K2200-08DUP	S	Reactive CN	P	0.0828 µg/l	4/24/2019 15:07:50
K2200-10	S	Reactive CN	P	0.2332 µg/l	4/24/2019 15:07:51
K2542-16	S	Reactive CN	P	0.1305 µg/l	4/24/2019 15:07:52
K2542-20	S	Reactive CN	P	0.2115 µg/l	4/24/2019 15:07:53
PB119154BL	S	Reactive CN	P	0.0586 µg/l	4/24/2019 15:07:54
K2204-04	S	Reactive CN	P	0.1338 µg/l	4/24/2019 15:07:55
K2204-04DUP	S	Reactive CN	P	0.2425 µg/l	4/24/2019 15:07:56
K2475-02	S	Reactive CN	P	0.1079 µg/l	4/24/2019 15:07:57
CCV5	S	Reactive CN	P	237.39 µg/l	4/24/2019 15:07:58
CCB5	S	Reactive CN	P	-0.2004 µg/l	4/24/2019 15:10:36