

2B102378

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : As

Instrument ID : Konelab

4/26/2019 12:21

Test: *Acetone*
~~Total~~ CN

ug/d

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.457	0.0	0.090	
ICB1	1.246	0.0	0.005	
CCV1	240.895	0.0	0.225	
CCB1	0.866	0.0	0.004	
PB119254BL	0.869	0.0	0.004	
K2198-08	0.904	0.0	0.004	
K2198-08DUP	0.729	0.0	0.004	
PB119253BL	0.713	0.0	0.004	
K2578-02	0.725	0.0	0.004	
K2578-02DUP	0.907	0.0	0.004	
CCV2	238.305	0.0	0.223	
CCB2	0.223	0.0	0.004	

N 12
Mean 48.320
SD 93.1969
CV% 192.88

Aquakem v. 7.2AQ1
Results from time period:
Fri Apr 26 10:05:58 2019
Fri Apr 26 12:20:43 2019

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	Reactive CN	P	0.3344	µg/l	4/26/2019 10:05:58
5.OPPBCN	A	Reactive CN	P	5.5783	µg/l	4/26/2019 10:05:59
10PPBCN	A	Reactive CN	P	10.4928	µg/l	4/26/2019 10:06:00
50PPBCN	A	Reactive CN	P	49.206	µg/l	4/26/2019 10:06:01
100PPBCN	A	Reactive CN	P	99.5195	µg/l	4/26/2019 10:06:02
250PPBCN	A	Reactive CN	P	249.4184	µg/l	4/26/2019 10:06:03
500PPBCN	A	Reactive CN	P	500.4507	µg/l	4/26/2019 10:06:04
ICV1	S	Reactive CN	P	93.4568	µg/l	4/26/2019 12:17:55
ICB1	S	Reactive CN	P	1.2457	µg/l	4/26/2019 12:17:56
CCV1	S	Reactive CN	P	240.8949	µg/l	4/26/2019 12:17:57
CCB1	S	Reactive CN	P	0.8663	µg/l	4/26/2019 12:17:58
PB119254BL	S	Reactive CN	P	0.8687	µg/l	4/26/2019 12:17:59
K2198-08	S	Reactive CN	P	0.9037	µg/l	4/26/2019 12:18:00
K2198-08DUP	S	Reactive CN	P	0.7288	µg/l	4/26/2019 12:18:01
PB119253BL	S	Reactive CN	P	0.7129	µg/l	4/26/2019 12:18:02
K2578-02	S	Reactive CN	P	0.7247	µg/l	4/26/2019 12:18:03
K2578-02DUP	S	Reactive CN	P	0.9072	µg/l	4/26/2019 12:18:04
CCV2	S	Reactive CN	P	238.3045	µg/l	4/26/2019 12:18:05
CCB2	S	Reactive CN	P	0.2234	µg/l	4/26/2019 12:20:43

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AS

Instrument ID : Konelab

4/26/2019 10:13


Test Total CN

Accepted 4/26/2019 10:13

Factor 1086
 Bias 0.004

Coeff. of det. 0.999990

Errors

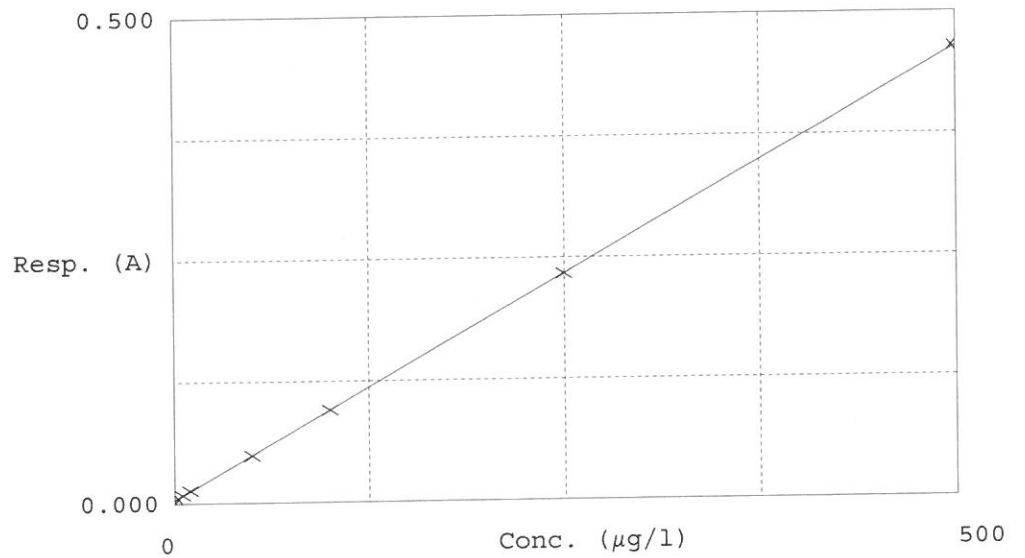

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.3344	0.0000	
2	5.0PPBCN	0.009	5.5783	5.0000	
3	10PPBCN	0.013	10.4928	10.0000	
4	50PPBCN	0.049	49.2060	50.0000	
5	100PPBCN	0.095	99.5195	100.0000	
6	250PPBCN	0.233	249.4184	250.0000	
7	500PPBCN	0.465	500.4507	500.0000	