

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/29/2019 14:53

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.217	0.0	0.095	
ICB1	0.949	0.0	0.005	
CCV1	241.955	0.0	0.234	
CCB1	0.954	0.0	0.005	
PB119290BL	0.720	0.0	0.004	
PB119290BS	98.672	0.0	0.098	
LOWPB119290	10.701	0.0	0.014	
HIGHPB119290	493.019	0.0	0.473	
K2551-04	836.155	0.0	0.799	Test limit high
K2601-01	13.242	0.0	0.016	
K2601-01DUP	12.370	0.0	0.016	
K2601-01MS	54.069	0.0	0.055	
K2601-01MSD	54.049	0.0	0.055	
CCV2	248.143	0.0	0.240	
CCB2	0.497	0.0	0.004	
K2551-04DLX2	417.886	0.0	0.401	
CCV3	251.074	0.0	0.243	
CCB3	0.710	0.0	0.004	

N	18
Mean	157.299
SD	227.5080
CV%	144.63

Aquakem v. 7.2AQ1

Results from time period:

Mon Apr 29 13:00:56 2019

Mon Apr 29 14:50:43 2019

AS

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.5758	µg/l	4/29/2019 13:38:02	
5.0PPBCN	A	Total CN	P	4.8647	µg/l	4/29/2019 13:38:03	
10PPBCN	A	Total CN	P	9.8703	µg/l	4/29/2019 13:38:04	
50PPBCN	A	Total CN	P	48.5529	µg/l	4/29/2019 13:38:05	
100PPBCN	A	Total CN	P	100.9619	µg/l	4/29/2019 13:38:06	
250PPBCN	A	Total CN	P	250.4363	µg/l	4/29/2019 13:38:07	
500PPBCN	A	Total CN	P	499.7381	µg/l	4/29/2019 13:38:08	
ICV1	S	Total CN	P	96.2174	µg/l	4/29/2019 14:03:22	
ICB1	S	Total CN	P	0.9495	µg/l	4/29/2019 14:03:23	
CCV1	S	Total CN	P	241.9546	µg/l	4/29/2019 14:03:24	
CCB1	S	Total CN	P	0.9536	µg/l	4/29/2019 14:03:25	
PB119290BL	S	Total CN	P	0.7205	µg/l	4/29/2019 14:03:26	
PB119290BS	S	Total CN	P	98.6724	µg/l	4/29/2019 14:03:27	
LOWPB119290	S	Total CN	P	10.7006	µg/l	4/29/2019 14:03:28	
HIGHPB119290	S	Total CN	P	493.0189	µg/l	4/29/2019 14:03:29	
K2551-04	S	Total CN	P	836.1555	µg/l	4/29/2019 14:03:30	
K2601-01	S	Total CN	P	13.2423	µg/l	4/29/2019 14:03:31	
K2601-01DUP	S	Total CN	P	12.37	µg/l	4/29/2019 14:03:32	
K2601-01MS	S	Total CN	P	54.0694	µg/l	4/29/2019 14:09:37	
K2601-01MSD	S	Total CN	P	54.0493	µg/l	4/29/2019 14:09:38	
CCV2	S	Total CN	P	248.1433	µg/l	4/29/2019 14:09:39	
CCB2	S	Total CN	P	0.4971	µg/l	4/29/2019 14:09:40	
K2551-04DLX2	S	Total CN	P	417.8857	µg/l	4/29/2019 14:34:52	
CCV3	S	Total CN	P	251.0742	µg/l	4/29/2019 14:34:55	
CCB3	S	Total CN	P	0.71	µg/l	4/29/2019 14:34:56	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/29/2019 13:38


Test Total CN

Accepted 4/29/2019 13:38

Factor 1051
Bias 0.004

Coeff. of det. 0.999982

Errors

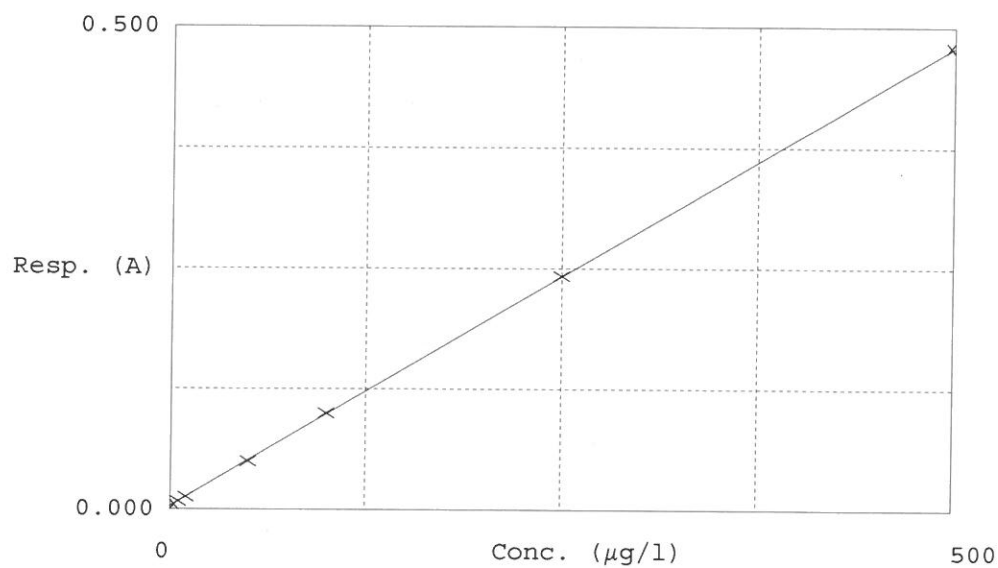

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.5758	0.0000	
2	5.0PPBCN	0.008	4.8647	5.0000	
3	10PPBCN	0.013	9.8703	10.0000	
4	50PPBCN	0.050	48.5529	50.0000	
5	100PPBCN	0.100	100.9619	100.0000	
6	250PPBCN	0.242	250.4363	250.0000	
7	500PPBCN	0.479	499.7381	500.0000	