

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/30/2019 15:14

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.269	0.0	0.100	
ICB1	-0.179	0.0	0.004	
CCV1	244.631	0.0	0.248	
CCB1	-0.141	0.0	0.005	
PB119292BL	-0.285	0.0	0.004	
PB119292BS	97.379	0.0	0.101	
MIDPB119292	246.181	0.0	0.249	
K2572-01	0.458	0.0	0.005	
K2572-01DUP	0.240	0.0	0.005	
K2572-01MS	29.068	0.0	0.034	
K2572-01MSD	28.980	0.0	0.033	
CCV2	256.147	0.0	0.259	
CCB2	-0.282	0.0	0.004	

N	13
Mean	76.805
SD	104.0068
CV%	135.42

Aquakem v. 7.2AQ1

Results from time period:

Tue Apr 30 15:08:51 2019

Tue Apr 30 15:13:13 2019

AS

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.6931	µg/l	4/30/2019 12:01:36	
5.0PPBCN	A	Total CN	P	4.5664	µg/l	4/30/2019 12:01:37	
10PPBCN	A	Total CN	P	9.7184	µg/l	4/30/2019 12:01:38	
50PPBCN	A	Total CN	P	50.0422	µg/l	4/30/2019 12:01:39	
100PPBCN	A	Total CN	P	100.1527	µg/l	4/30/2019 12:01:40	
250PPBCN	A	Total CN	P	252.4765	µg/l	4/30/2019 12:01:41	
500PPBCN	A	Total CN	P	498.737	µg/l	4/30/2019 12:01:42	
ICV1	S	Total CN	P	96.2686	µg/l	4/30/2019 15:08:51	
ICB1	S	Total CN	P	-0.1791	µg/l	4/30/2019 15:08:52	
CCV1	S	Total CN	P	244.6313	µg/l	4/30/2019 15:08:53	
CCB1	S	Total CN	P	-0.1409	µg/l	4/30/2019 15:08:54	
PB119292BL	S	Total CN	P	-0.2846	µg/l	4/30/2019 15:08:55	
PB119292BS	S	Total CN	P	97.3792	µg/l	4/30/2019 15:08:56	
MIDPB119292	S	Total CN	P	246.181	µg/l	4/30/2019 15:08:57	
K2572-01	S	Total CN	P	0.4581	µg/l	4/30/2019 15:08:58	
K2572-01DUP	S	Total CN	P	0.2398	µg/l	4/30/2019 15:08:59	
K2572-01MS	S	Total CN	P	29.0683	µg/l	4/30/2019 15:09:00	
K2572-01MSD	S	Total CN	P	28.9804	µg/l	4/30/2019 15:09:01	
CCV2	S	Total CN	P	256.1468	µg/l	4/30/2019 15:13:12	
CCB2	S	Total CN	P	-0.2823	µg/l	4/30/2019 15:13:13	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

4/30/2019 15:09


Test Total CN

Accepted 4/30/2019 12:13

Factor 1006
Bias 0.005

Coeff. of det. 0.999959

Errors

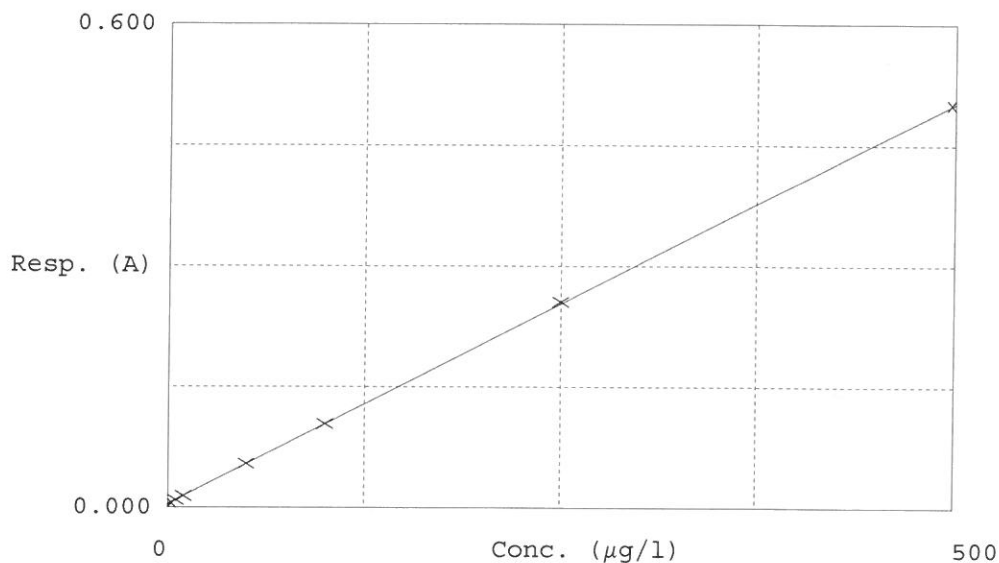

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.6931	0.0000	
2	5.0PPBCN	0.009	4.5664	5.0000	
3	10PPBCN	0.014	9.7184	10.0000	
4	50PPBCN	0.054	50.0422	50.0000	
5	100PPBCN	0.104	100.1527	100.0000	
6	250PPBCN	0.256	252.4765	250.0000	
7	500PPBCN	0.500	498.7370	500.0000	