

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/1/2019 11:14

Test: *Dechlorine* Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.084	0.0	0.100	
ICB1	0.165	0.0	0.005	
CCV1	244.553	0.0	0.245	
CCB1	-0.132	0.0	0.005	
PB119359BL	-0.457	0.0	0.004	
K2191-04	-0.595	0.0	0.004	
K2191-04DUP	-0.312	0.0	0.004	
K2204-06	-0.283	0.0	0.004	
K2617-03	-0.646	0.0	0.004	
PB119360BL	-0.465	0.0	0.004	
K2617-05	-0.434	0.0	0.004	
K2617-05DUP	-0.685	0.0	0.004	
K2621-02	-0.733	0.0	0.004	
BLK	-0.729	0.0	0.004	
CCV2	255.508	0.0	0.256	
CCB2	-0.333	0.0	0.004	

N	16
Mean	36.969
SD	86.6610
CV%	234.41

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/1/2019 7:58


Test Total CN

Accepted 5/1/2019 7:58

Factor 1018
Bias 0.005

Coeff. of det. 0.999973

Errors

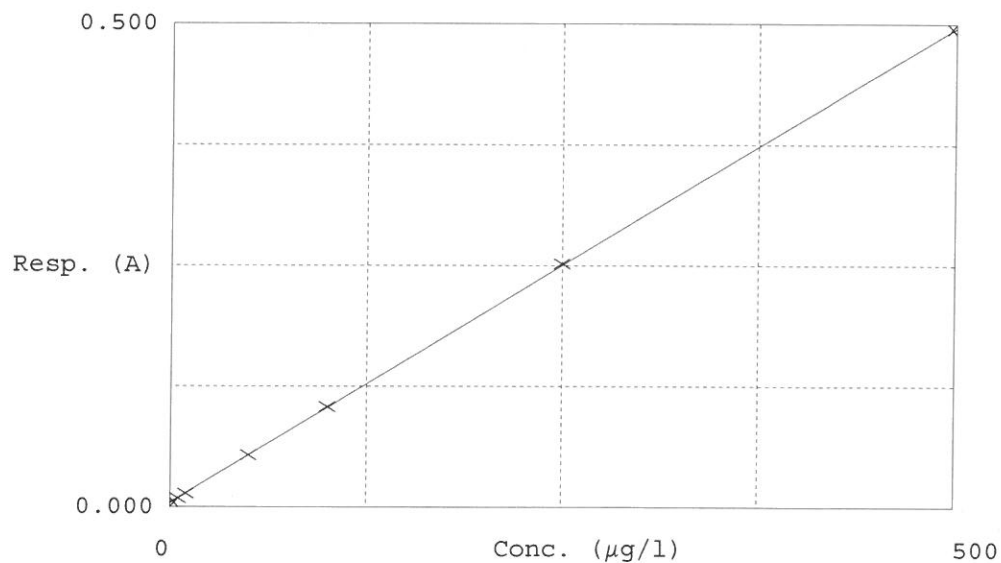

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.6951	0.0000	
2	5.0PPBCN	0.009	4.4760	5.0000	
3	10PPBCN	0.014	9.6143	10.0000	
4	50PPBCN	0.054	50.0799	50.0000	
5	100PPBCN	0.104	100.8185	100.0000	
6	250PPBCN	0.252	251.7304	250.0000	
7	500PPBCN	0.495	498.9761	500.0000	

AS

Aquakem v. 7.2AQ1

Results from time period:

Wed May 01 11:08:59 2019

Wed May 01 11:13:50 2019

Sample Id	Sam/Ctr/c/	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.6951	µg/l	5/1/2019 7:57:59	
5.OPPBCN	A	Reactive CN	P	4.476	µg/l	5/1/2019 7:58:00	
10PPBCN	A	Reactive CN	P	9.6143	µg/l	5/1/2019 7:58:01	
50PPBCN	A	Reactive CN	P	50.0799	µg/l	5/1/2019 7:58:02	
100PPBCN	A	Reactive CN	P	100.8185	µg/l	5/1/2019 7:58:03	
250PPBCN	A	Reactive CN	P	251.7304	µg/l	5/1/2019 7:58:04	
500PPBCN	A	Reactive CN	P	498.9761	µg/l	5/1/2019 7:58:05	
ICV1	S	Reactive CN	P	97.0843	µg/l	5/1/2019 11:08:59	
ICB1	S	Reactive CN	P	0.1652	µg/l	5/1/2019 11:09:00	
CCV1	S	Reactive CN	P	244.5535	µg/l	5/1/2019 11:09:01	
CCB1	S	Reactive CN	P	-0.1317	µg/l	5/1/2019 11:09:02	
PB119359BL	S	Reactive CN	P	-0.4571	µg/l	5/1/2019 11:09:03	
K2191-04	S	Reactive CN	P	-0.5945	µg/l	5/1/2019 11:09:04	
K2191-04DUP	S	Reactive CN	P	-0.3121	µg/l	5/1/2019 11:09:05	
K2204-06	S	Reactive CN	P	-0.2828	µg/l	5/1/2019 11:09:06	
K2617-03	S	Reactive CN	P	-0.6462	µg/l	5/1/2019 11:09:07	
PB119360BL	S	Reactive CN	P	-0.4654	µg/l	5/1/2019 11:09:08	
K2617-05	S	Reactive CN	P	-0.4343	µg/l	5/1/2019 11:09:09	
K2617-05DUP	S	Reactive CN	P	-0.6855	µg/l	5/1/2019 11:13:46	
K2621-02	S	Reactive CN	P	-0.7334	µg/l	5/1/2019 11:13:47	
CCV2	S	Reactive CN	P	255.5079	µg/l	5/1/2019 11:13:49	
CCB2	S	Reactive CN	P	-0.3332	µg/l	5/1/2019 11:13:50	