


LB102497

7470A

INSTRUMENT ID: C01

Linear

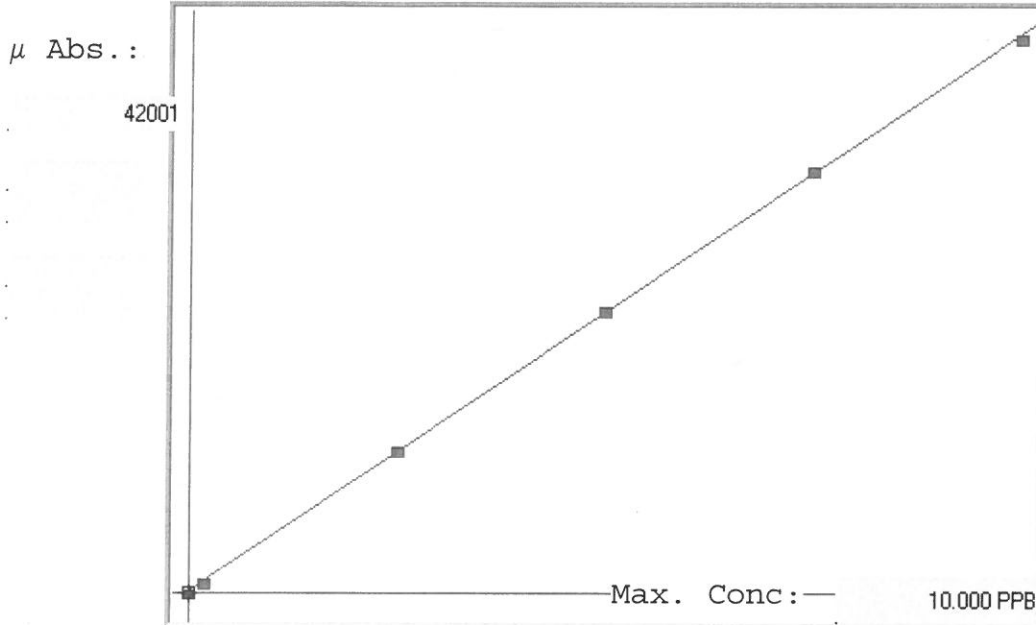

A= 0.0000e+000

B= 2.3688e-004

C= -3.2341e-002

Rho= 0.9998919

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.029	-0.029	13	0.000	13				
0.2	0.200	0.159	-0.041	807	0.0 %	807				
2.5	2.500	2.535	0.035	10839	0.0 %	10839				
5.0	5.000	5.062	0.062	21504	0.0 %	21504				
7.5	7.500	7.556	0.056	32036	0.0 %	32036				
10.0	10.000	9.917	-0.083	42001	0.0 %	42001				

LB102497 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 02 May 2019 10:55:03

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	S0-0	13	-	0.0000	7470A	PPB	02 May 2019 10:56:49	S	Std
0.2 - 1	S0-2	807	-	0.2000	7470A	PPB	02 May 2019 10:58:57	S	Std
2.5 - 1	S2-5	10839	-	2.5000	7470A	PPB	02 May 2019 11:01:05	S	Std
5.0 - 1	S5-0	21504	-	5.0000	7470A	PPB	02 May 2019 11:03:13	S	Std
7.5 - 1	S7-5	32036	-	7.5000	7470A	PPB	02 May 2019 11:05:21	S	Std
10.0 - 1	S10-0	42001	-	10.0000	7470A	PPB	02 May 2019 11:11:50	S	Std
ICV26 - 1	ICV26	17133	4.0262	-	7470A	PPB	02 May 2019 11:15:44	U	SMPL
ICB26 - 1	ICB26	56	-0.0191	-	7470A	PPB	02 May 2019 11:17:51	U	SMPL
CCV22 - 1	CCV22	21083	4.9619	-	7470A	PPB	02 May 2019 11:19:56	U	SMPL
CCB22 - 1	CCB22	-60	-0.0466	-	7470A	PPB	02 May 2019 11:22:02	U	SMPL
CRA - 1	CRA	823	0.1626	-	7470A	PPB	02 May 2019 11:24:08	U	SMPL
HighStd - 1	HighStd	41151	9.7157	-	7470A	PPB	02 May 2019 11:26:14	U	SMPL
ChkStd - 1	ChkStd	29993	7.0725	-	7470A	PPB	02 May 2019 11:28:21	U	SMPL
PB119381BL - 1	PBW	-93	-0.0544	-	7470A	PPB	02 May 2019 11:30:29	U	SMPL
PB119381BS - 1	LCSW	16254	3.8180	-	7470A	PPB	02 May 2019 11:32:35	U	SMPL
K2617-04 - 1	SUMP-PIT	4363	1.0012	-	7470A	PPB	02 May 2019 11:34:43	U	SMPL
K2621-01 - 1	A5327	9	-0.0302	-	7470A	PPB	02 May 2019 11:36:50	U	SMPL
K2621-01DUP - 1	A5327DUP	70	-0.0158	-	7470A	PPB	02 May 2019 11:38:58	U	SMPL
K2621-01MS - 1	A5327MS	18390	4.3240	-	7470A	PPB	02 May 2019 11:41:06	U	SMPL
K2621-01MSD - 1	A5327MSD	18492	4.3481	-	7470A	PPB	02 May 2019 11:43:12	U	SMPL
CCV23 - 1	CCV23	21090	4.9636	-	7470A	PPB	02 May 2019 11:45:19	U	SMPL
CCB23 - 1	CCB23	-62	-0.0470	-	7470A	PPB	02 May 2019 11:47:26	U	SMPL
K2650-01 - 1	GROUND-WATER	26	-0.0262	-	7470A	PPB	02 May 2019 11:49:32	U	SMPL
K2653-01 - 1	MR-SUMP-PIT	346	0.0496	-	7470A	PPB	02 May 2019 11:51:39	U	SMPL
PB119382BL - 1	PBW	-7	-0.0340	-	7470A	PPB	02 May 2019 11:53:46	U	SMPL
PB119382BS - 1	LCSW	16438	3.8616	-	7470A	PPB	02 May 2019 11:55:53	U	SMPL
K2191-04 - 1	P-66-TP	11	-0.0297	-	7470A	PPB	02 May 2019 11:58:00	U	SMPL
K2204-06 - 1	TR-04-043019	-13	-0.0354	-	7470A	PPB	02 May 2019 12:00:07	U	SMPL
K2204-06DUP - 1	TR-04-043019DUP	17	-0.0283	-	7470A	PPB	02 May 2019 12:02:14	U	SMPL
K2204-06MS - 1	TR-04-043019MS	17802	4.1847	-	7470A	PPB	02 May 2019 12:04:22	U	SMPL
K2204-06MSD - 1	TR-04-043019MSD	17961	4.2223	-	7470A	PPB	02 May 2019 12:06:30	U	SMPL
K2617-03 - 1	ROCK-COMP	16	-0.0286	-	7470A	PPB	02 May 2019 12:08:37	U	SMPL
CCV24 - 1	CCV24	21521	5.0657	-	7470A	PPB	02 May 2019 12:10:43	U	SMPL
CCB24 - 1	CCB24	-60	-0.0466	-	7470A	PPB	02 May 2019 12:12:50	U	SMPL
K2619-01 - 1	DRUM-1-4-A	-6	-0.0338	-	7470A	PPB	02 May 2019 12:14:57	U	SMPL
K2619-02 - 1	DRUM-1-5-B	-19	-0.0368	-	7470A	PPB	02 May 2019 12:17:04	U	SMPL
K2623-03 - 1	SP-1	-25	-0.0383	-	7470A	PPB	02 May 2019 12:19:11	U	SMPL
PB119383BL - 1	PBW	10	-0.0300	-	7470A	PPB	02 May 2019 12:21:18	U	SMPL
PB119383BS - 1	LCSW	16565	3.8917	-	7470A	PPB	02 May 2019 12:23:25	U	SMPL
K2617-05 - 1	SUMP-PIT	-14	-0.0357	-	7470A	PPB	02 May 2019 12:25:33	U	SMPL
K2621-02 - 1	A5327	7	-0.0307	-	7470A	PPB	02 May 2019 12:27:41	U	SMPL
K2621-02DUP - 1	A5327DUP	12	-0.0295	-	7470A	PPB	02 May 2019 12:29:50	U	SMPL
K2621-02MS - 1	A5327MS	17863	4.1991	-	7470A	PPB	02 May 2019 12:31:58	U	SMPL
K2621-02MSD - 1	A5327MSD	17648	4.1482	-	7470A	PPB	02 May 2019 12:34:05	U	SMPL
CCV25 - 1	CCV25	22638	5.3303	-	7470A	PPB	02 May 2019 12:36:11	U	SMPL
CCB25 - 1	CCB25	-52	-0.0447	-	7470A	PPB	02 May 2019 12:38:18	U	SMPL
PB119382TB - 1	PB119346TB	-2	-0.0328	-	7470A	PPB	02 May 2019 12:40:25	U	SMPL
PB119383TB - 1	PB119351TB	8	-0.0304	-	7470A	PPB	02 May 2019 12:42:31	U	SMPL
K2621-01LX5 - 1		8	-0.0304	-	7470A	PPB	02 May 2019 12:44:37	U	SMPL
K2621-01A - 1		18627	4.3801	-	7470A	PPB	02 May 2019 12:46:44	U	SMPL
K2204-06LX5 - 1		-46	-0.0432	-	7470A	PPB	02 May 2019 12:48:55	U	SMPL
K2204-06A - 1		18124	4.2610	-	7470A	PPB	02 May 2019 12:51:05	U	SMPL
K2621-02LX5 - 1		-23	-0.0378	-	7470A	PPB	02 May 2019 12:53:12	U	SMPL
K2621-02A - 1		17526	4.1193	-	7470A	PPB	02 May 2019 12:55:22	U	SMPL
CCV26 - 1	CCV26	21147	4.9771	-	7470A	PPB	02 May 2019 12:57:30	U	SMPL
CCB26 - 1	CCB26	-46	-0.0432	-	7470A	PPB	02 May 2019 12:59:37	U	SMPL