

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/6/2019 10:59

Test: Phenolics-

Sample Id	Result ^{mg/L}	Dil. 1 +	Response	Errors
ICV1	1.055	0.0	0.127	
ICB1	0.003	0.0	0.016	
CCV1	1.042	0.0	0.126	
CCB1	0.009	0.0	0.017	
PB119466BL	0.002	0.0	0.016	
PB119466BS	1.055	0.0	0.127	
K2668-01	-0.001	0.0	0.016	
K2668-01DUP	-0.002	0.0	0.016	
K2668-01MS	0.863	0.0	0.107	
K2668-01MSD	0.861	0.0	0.107	
K2668-03	0.003	0.0	0.016	
K2668-05	0.001	0.0	0.016	
CCV2	1.041	0.0	0.126	
CCB2	-0.011	0.0	0.015	

N 14
Mean 0.423
SD 0.5098
CV% 120.55

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/6/2019 10:30


Test Phenolics-

Accepted 5/6/2019 10:30

Factor 9.477
Bias 0.016

Coeff. of det. 0.999991

Errors

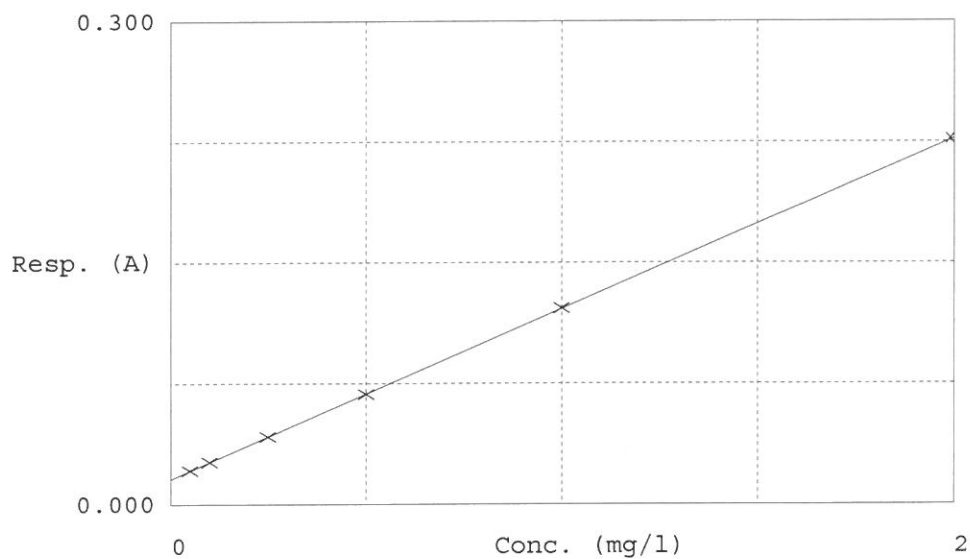

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.021	0.0505	0.0500	
2	Phenol-2	0.026	0.1001	0.1000	
3	Phenol-2	0.042	0.2496	0.2500	
4	Phenol-2	0.068	0.4972	0.5000	
5	Phenol-2	0.122	1.0038	1.0000	
6	Phenol-2	0.227	1.9988	2.0000	

A>

Aquamem v. 7.2AQ1

Results from time period:

Mon May 06 10:30:06 2019

Mon May 06 10:58:38 2019

Sample Id	Sam/Ctr/c/	Test short na	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0505	mg/l	5/6/2019 10:30:06	
0.1PPM	A	Phenolics-	P	0.1001	mg/l	5/6/2019 10:30:07	
0.25PPM	A	Phenolics-	P	0.2496	mg/l	5/6/2019 10:30:08	
0.50PPM	A	Phenolics-	P	0.4972	mg/l	5/6/2019 10:30:09	
1.0PPM	A	Phenolics-	P	1.0038	mg/l	5/6/2019 10:30:10	
2.0PPM	A	Phenolics-	P	1.9988	mg/l	5/6/2019 10:30:11	
ICV1	S	Phenolics-	P	1.0549	mg/l	5/6/2019 10:53:41	
ICB1	S	Phenolics-	P	0.0026	mg/l	5/6/2019 10:53:42	
CCV1	S	Phenolics-	P	1.0419	mg/l	5/6/2019 10:53:43	
CCB1	S	Phenolics-	P	0.0086	mg/l	5/6/2019 10:53:44	
PB119466BL	S	Phenolics-	P	0.0021	mg/l	5/6/2019 10:53:45	
PB119466BS	S	Phenolics-	P	1.0551	mg/l	5/6/2019 10:53:46	
K2668-01	S	Phenolics-	P	-0.0012	mg/l	5/6/2019 10:53:47	
K2668-01DUP	S	Phenolics-	P	-0.0021	mg/l	5/6/2019 10:53:48	
K2668-01MS	S	Phenolics-	P	0.8633	mg/l	5/6/2019 10:53:49	
K2668-01MSD	S	Phenolics-	P	0.8612	mg/l	5/6/2019 10:53:50	
K2668-03	S	Phenolics-	P	0.003	mg/l	5/6/2019 10:53:51	
K2668-05	S	Phenolics-	P	0.0009	mg/l	5/6/2019 10:53:52	
CCV2	S	Phenolics-	P	1.0411	mg/l	5/6/2019 10:58:37	
CCB2	S	Phenolics-	P	-0.0107	mg/l	5/6/2019 10:58:38	