

LB102589


7470A

INSTRUMENT ID : CU1

Linear

 μ Abs.:

41277

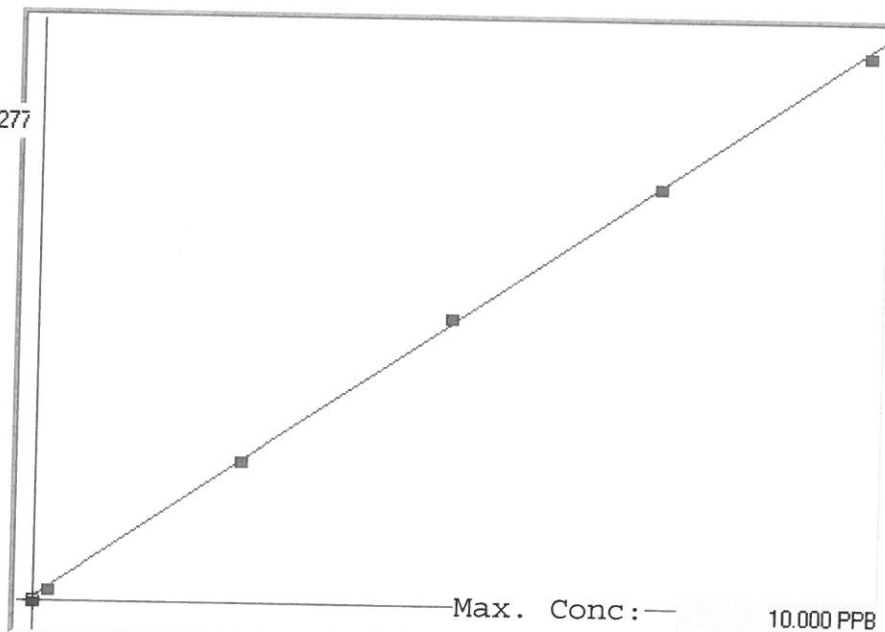

A= 0.0000e+000

B= 2.4185e-004

C= -6.6206e-002

Rho= 0.9998259

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.044	-0.044	92	0.000	92				
0.2	0.200	0.167	-0.033	965	0.0 %	965				
2.5	2.500	2.510	0.010	10654	0.0 %	10654				
5.0	5.000	5.135	0.135	21505	0.0 %	21505				
7.5	7.500	7.515	0.015	31345	0.0 %	31345				
10.0	10.000	9.917	-0.083	41277	0.0 %	41277				

LB102589 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 07 May 2019 12:46:34

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	92	-	0.00007470A	PPB		07 May 2019 12:49:26	S	Std
0.2 - 1	50.2	965	-	0.20007470A	PPB		07 May 2019 12:51:34	S	Std
2.5 - 1	52.5	10654	-	2.50007470A	PPB		07 May 2019 12:53:43	S	Std
5.0 - 1	55.0	21505	-	5.00007470A	PPB		07 May 2019 12:55:52	S	Std
7.5 - 1	57.5	31345	-	7.50007470A	PPB		07 May 2019 12:57:59	S	Std
10.0 - 1	510.0	41277	-	10.00007470A	PPB		07 May 2019 13:00:06	S	Std
ICV31 - 1	ICV31	16835	4.0054	-7470A	PPB		07 May 2019 13:04:09	U	SMPL
ICB31 - 1	ICB31	26	-0.0599	-7470A	PPB		07 May 2019 13:06:16	U	SMPL
CCV45 - 1	CCV45	20642	4.9261	-7470A	PPB		07 May 2019 13:08:22	U	SMPL
CCB45 - 1	CCB45	15	-0.0626	-7470A	PPB		07 May 2019 13:10:28	U	SMPL
CRA - 1	CRA	958	0.1655	-7470A	PPB		07 May 2019 13:12:34	U	SMPL
HighStd - 1	HighStd	40794	9.7999	-7470A	PPB		07 May 2019 13:14:40	U	SMPL
ChkStd - 1	ChkStd	28699	6.8747	-7470A	PPB		07 May 2019 13:16:46	U	SMPL
PB119524BL - 1	PBW	56	-0.0527	-7470A	PPB		07 May 2019 13:18:54	U	SMPL
PB119524BS - 1	LCSW	17398	4.1416	-7470A	PPB		07 May 2019 13:21:01	U	SMPL
K2672-02 - 1	SB-01-COMP	96	-0.0430	-7470A	PPB		07 May 2019 13:23:09	U	SMPL
K2672-02DUP - 1	SB-01-COMPDUP	118	-0.0377	-7470A	PPB		07 May 2019 13:25:16	U	SMPL
K2672-02MS - 1	SB-01-COMPMS	17749	4.2264	-7470A	PPB		07 May 2019 13:27:25	U	SMPL
K2672-02MSD - 1	SB-01-COMPMSD	17521	4.1713	-7470A	PPB		07 May 2019 13:29:32	U	SMPL
K2672-04 - 1	SB-02-COMP	103	-0.0413	-7470A	PPB		07 May 2019 13:31:39	U	SMPL
CCV46 - 1	CCV46	20165	4.8108	-7470A	PPB		07 May 2019 13:33:44	U	SMPL
CCB46 - 1	CCB46	19	-0.0616	-7470A	PPB		07 May 2019 13:35:51	U	SMPL
K2672-06 - 1	SB-03-COMP	157	-0.0282	-7470A	PPB		07 May 2019 13:37:58	U	SMPL
K2672-08 - 1	SB-04-COMP	174	-0.0241	-7470A	PPB		07 May 2019 13:40:03	U	SMPL
K2672-10 - 1	SB-05-COMP	182	-0.0222	-7470A	PPB		07 May 2019 13:42:10	U	SMPL
K2672-12 - 1	SB-06-COMP	180	-0.0227	-7470A	PPB		07 May 2019 13:44:17	U	SMPL
K2672-14 - 1	SB-07-COMP	142	-0.0319	-7470A	PPB		07 May 2019 13:46:24	U	SMPL
K2672-16 - 1	SB-08-COMP	122	-0.0367	-7470A	PPB		07 May 2019 13:48:31	U	SMPL
K2672-18 - 1	SB-09-COMP	131	-0.0345	-7470A	PPB		07 May 2019 13:50:38	U	SMPL
K2672-20 - 1	SB-10-COMP	137	-0.0331	-7470A	PPB		07 May 2019 13:52:46	U	SMPL
K2673-02 - 1	SB-11-COMP	135	-0.0336	-7470A	PPB		07 May 2019 13:54:54	U	SMPL
K2673-04 - 1	SB-12-COMP	124	-0.0362	-7470A	PPB		07 May 2019 13:57:01	U	SMPL
CCV47 - 1	CCV47	20325	4.8495	-7470A	PPB		07 May 2019 13:59:08	U	SMPL
CCB47 - 1	CCB47	30	-0.0590	-7470A	PPB		07 May 2019 14:01:15	U	SMPL
K2673-06 - 1	SB-13-COMP	128	-0.0352	-7470A	PPB		07 May 2019 14:03:22	U	SMPL
K2673-08 - 1	SB-14-COMP	162	-0.0270	-7470A	PPB		07 May 2019 14:05:29	U	SMPL
K2673-10 - 1	SB-15-COMP	174	-0.0241	-7470A	PPB		07 May 2019 14:07:35	U	SMPL
K2673-12 - 1	SB-16-COMP	163	-0.0268	-7470A	PPB		07 May 2019 14:09:42	U	SMPL
K2673-14 - 1	SB-17-COMP	159	-0.0278	-7470A	PPB		07 May 2019 14:11:48	U	SMPL
K2673-15 - 1	SP-01-COMP	237	-0.0089	-7470A	PPB		07 May 2019 14:13:56	U	SMPL
K2673-16 - 1	SP-02-COMP	181	-0.0224	-7470A	PPB		07 May 2019 14:16:03	U	SMPL
PB119525BL - 1	PBW	190	-0.0203	-7470A	PPB		07 May 2019 14:18:11	U	SMPL
PB119525BS - 1	LCSW	17769	4.2313	-7470A	PPB		07 May 2019 14:20:19	U	SMPL
K2674-04 - 1	SV28545L	156	-0.0285	-7470A	PPB		07 May 2019 14:22:26	U	SMPL
CCV48 - 1	CCV48	22208	5.3049	-7470A	PPB		07 May 2019 14:24:35	U	SMPL
CCB48 - 1	CCB48	53	-0.0534	-7470A	PPB		07 May 2019 14:26:43	U	SMPL
K2696-02 - 1	WC-20190502	161	-0.0273	-7470A	PPB		07 May 2019 14:28:51	U	SMPL
K2696-02DUP - 1	WC-20190502DUP	168	-0.0256	-7470A	PPB		07 May 2019 14:30:58	U	SMPL
K2696-02MS - 1	WC-20190502MS	18035	4.2956	-7470A	PPB		07 May 2019 14:33:04	U	SMPL
K2696-02MSD - 1	WC-20190502MSD	17711	4.2173	-7470A	PPB		07 May 2019 14:35:11	U	SMPL
PB119526BL - 1	PBW	105	-0.0408	-7470A	PPB		07 May 2019 14:37:18	U	SMPL
PB119526BS - 1	LCSW	17854	4.2518	-7470A	PPB		07 May 2019 14:39:25	U	SMPL
K2639-02 - 1	NB-08-050319-A	128	-0.0352	-7470A	PPB		07 May 2019 14:41:32	U	SMPL
K2639-02DUP - 1	NB-08-050319-ADUP	166	-0.0261	-7470A	PPB		07 May 2019 14:43:41	U	SMPL
K2639-02MS - 1	NB-08-050319-AMS	17574	4.1841	-7470A	PPB		07 May 2019 14:45:49	U	SMPL
K2639-02MSD - 1	NB-08-050319-AMSD	17473	4.1597	-7470A	PPB		07 May 2019 14:47:55	U	SMPL
CCV49 - 1	CCV49	22494	5.3740	-7470A	PPB		07 May 2019 14:50:02	U	SMPL
CCB49 - 1	CCB49	26	-0.0599	-7470A	PPB		07 May 2019 14:52:18	U	SMPL
K2639-04 - 1	NB-08-050319-B	229	-0.0108	-7470A	PPB		07 May 2019 14:54:27	U	SMPL
K2680-01 - 1	SSSI-0502-S-TCLP-8	149	-0.0302	-7470A	PPB		07 May 2019 14:56:34	U	SMPL
K2680-02 - 1	SSSI-0502-S-TCLP-9	158	-0.0280	-7470A	PPB		07 May 2019 14:58:40	U	SMPL
K2680-03 - 1	SSSI-0502-S-TCLP-10	145	-0.0311	-7470A	PPB		07 May 2019 15:00:47	U	SMPL
PB119524TB - 1	PB119447TB	153	-0.0292	-7470A	PPB		07 May 2019 15:02:55	U	SMPL
PB119525TB - 1	PB119448TB	152	-0.0294	-7470A	PPB		07 May 2019 15:05:01	U	SMPL
PB119526TB - 1	PB119462TB	142	-0.0319	-7470A	PPB		07 May 2019 15:07:09	U	SMPL
K2672-02LX5 - 1		132	-0.0343	-7470A	PPB		07 May 2019 15:09:17	U	SMPL
K2672-02A - 1		17885	4.2593	-7470A	PPB		07 May 2019 15:11:25	U	SMPL
K2696-02LX5 - 1		114	-0.0386	-7470A	PPB		07 May 2019 15:13:33	U	SMPL
CCV50 - 1	CCV50	22280	5.3223	-7470A	PPB		07 May 2019 15:15:40	U	SMPL
CCB50 - 1	CCB50	42	-0.0560	-7470A	PPB		07 May 2019 15:17:47	U	SMPL
K2696-02A - 1		17721	4.2197	-7470A	PPB		07 May 2019 15:19:54	U	SMPL
K2639-02LX5 - 1		119	-0.0374	-7470A	PPB		07 May 2019 15:22:01	U	SMPL
K2639-02A - 1		17745	4.2255	-7470A	PPB		07 May 2019 15:24:08	U	SMPL
CCV51 - 1	CCV51	20742	4.9503	-7470A	PPB		07 May 2019 15:26:15	U	SMPL
CCB51 - 1	CCB51	-1	-0.0664	-7470A	PPB		07 May 2019 15:28:22	U	SMPL