

AB/02671

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/10/2019 12:38

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	98.373	0.0	0.103	
ICB1	0.353	0.0	0.005	
CCV1	245.554	0.0	0.251	
CCB1	-0.117	0.0	0.004	
PB119627BL	0.080	0.0	0.004	
PB119627BS	99.552	0.0	0.104	
MIDPB119627	246.705	0.0	0.252	
K2675-01	0.051	0.0	0.004	
K2781-01	0.126	0.0	0.004	
K2781-01DUP	-0.034	0.0	0.004	
K2781-01MS	33.566	0.0	0.038	
K2781-01MSD	34.516	0.0	0.039	
CCV2	259.886	0.0	0.265	
CCB2	-0.075	0.0	0.004	

N	14
Mean	72.753
SD	102.4718
CV%	140.85

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/10/2019 12:09


Test Total CN

Accepted 5/10/2019 12:09

Factor 995.7
Bias 0.004

Coeff. of det. 0.999967

Errors

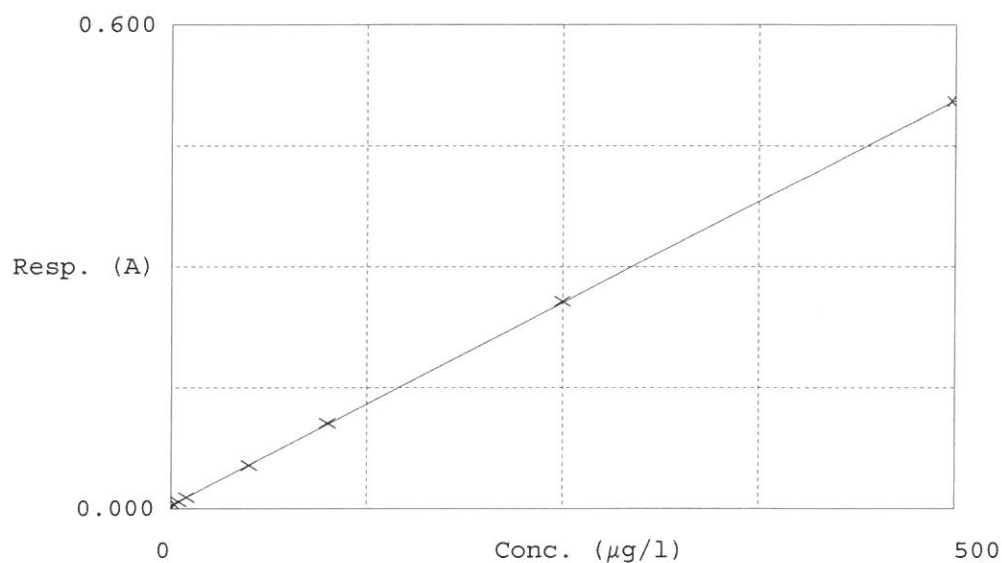

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.2793	0.0000	
2	5.0PPBCN	0.009	4.3408	5.0000	
3	10PPBCN	0.014	9.6349	10.0000	
4	50PPBCN	0.054	49.3677	50.0000	
5	100PPBCN	0.106	101.2120	100.0000	
6	250PPBCN	0.257	251.7782	250.0000	
7	500PPBCN	0.505	498.9456	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Fri May 10 10:58:33 2019

Fri May 10 12:37:47 2019

AS

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.2793	µg/l	5/10/2019 12:08:47	
5.0PPBCN	A	Total CN	P	4.3408	µg/l	5/10/2019 12:08:48	
10PPBCN	A	Total CN	P	9.6349	µg/l	5/10/2019 12:08:49	
50PPBCN	A	Total CN	P	49.3677	µg/l	5/10/2019 12:08:50	
100PPBCN	A	Total CN	P	101.212	µg/l	5/10/2019 12:08:51	
250PPBCN	A	Total CN	P	251.7782	µg/l	5/10/2019 12:08:52	
500PPBCN	A	Total CN	P	498.9456	µg/l	5/10/2019 12:08:53	
ICV1	S	Total CN	P	98.3734	µg/l	5/10/2019 12:33:25	
ICB1	S	Total CN	P	0.3531	µg/l	5/10/2019 12:33:26	
CCV1	S	Total CN	P	245.5543	µg/l	5/10/2019 12:33:27	
CCB1	S	Total CN	P	-0.1175	µg/l	5/10/2019 12:33:28	
PB119627BL	S	Total CN	P	0.0796	µg/l	5/10/2019 12:33:29	
PB119627BS	S	Total CN	P	99.5517	µg/l	5/10/2019 12:33:30	
MIDPB119627	S	Total CN	P	246.7052	µg/l	5/10/2019 12:33:31	
K2675-01	S	Total CN	P	0.051	µg/l	5/10/2019 12:33:32	
K2781-01	S	Total CN	P	0.126	µg/l	5/10/2019 12:33:33	
K2781-01DUP	S	Total CN	P	-0.0342	µg/l	5/10/2019 12:33:34	
K2781-01MS	S	Total CN	P	33.5664	µg/l	5/10/2019 12:33:35	
K2781-01MSD	S	Total CN	P	34.5165	µg/l	5/10/2019 12:37:44	
CCV2	S	Total CN	P	259.8864	µg/l	5/10/2019 12:37:45	
CCB2	S	Total CN	P	-0.0749	µg/l	5/10/2019 12:37:46	