

2B102680

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/10/2019 15:35

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	98.530	0.0	0.103	
ICB1	0.268	0.0	0.005	
CCV1	246.275	0.0	0.252	
CCB1	-0.077	0.0	0.004	
PB119634BL	0.369	0.0	0.005	
PB119634BS	98.731	0.0	0.103	
K2774-01	1.637	0.0	0.006	
K2774-01DUP	1.488	0.0	0.006	
K2774-01MS	33.550	0.0	0.038	
K2774-01MSD	33.657	0.0	0.038	
K2779-01	0.291	0.0	0.005	
K2779-03	0.774	0.0	0.005	
K2779-05	1.809	0.0	0.006	
K2801-01	0.902	0.0	0.005	
CCV2	248.152	0.0	0.254	
CCB2	-0.032	0.0	0.004	
K2801-04	0.256	0.0	0.005	
K2801-07	0.191	0.0	0.004	
CCV3	250.473	0.0	0.256	
CCB3	0.330	0.0	0.005	

N 20
Mean 50.879
SD 90.2976
CV% 177.48

Aquakem v. 7.2AQ1

Results from time period:

Fri May 10 15:27:49 2019

Fri May 10 15:35:05 2019

AS

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.2793	µg/l	5/10/2019 12:08:47	
5.0PPBCN	A	Total CN	P	4.3408	µg/l	5/10/2019 12:08:48	
10PPBCN	A	Total CN	P	9.6349	µg/l	5/10/2019 12:08:49	
50PPBCN	A	Total CN	P	49.3677	µg/l	5/10/2019 12:08:50	
100PPBCN	A	Total CN	P	101.212	µg/l	5/10/2019 12:08:51	
250PPBCN	A	Total CN	P	251.7782	µg/l	5/10/2019 12:08:52	
500PPBCN	A	Total CN	P	498.9456	µg/l	5/10/2019 12:08:53	
ICV1	S	Total CN	P	98.5304	µg/l	5/10/2019 15:27:49	
ICB1	S	Total CN	P	0.2676	µg/l	5/10/2019 15:27:50	
CCV1	S	Total CN	P	246.2754	µg/l	5/10/2019 15:27:51	
CCB1	S	Total CN	P	-0.0767	µg/l	5/10/2019 15:27:52	
PB119634BL	S	Total CN	P	0.3694	µg/l	5/10/2019 15:27:53	
PB119634BS	S	Total CN	P	98.7312	µg/l	5/10/2019 15:27:54	
K2774-01	S	Total CN	P	1.6372	µg/l	5/10/2019 15:27:55	
K2774-01DUP	S	Total CN	P	1.4875	µg/l	5/10/2019 15:27:56	
K2774-01MS	S	Total CN	P	33.5497	µg/l	5/10/2019 15:27:57	
K2774-01MSD	S	Total CN	P	33.6567	µg/l	5/10/2019 15:27:58	
K2779-01	S	Total CN	P	0.2915	µg/l	5/10/2019 15:27:59	
K2779-03	S	Total CN	P	0.7738	µg/l	5/10/2019 15:34:56	
K2779-05	S	Total CN	P	1.8086	µg/l	5/10/2019 15:34:57	
K2801-01	S	Total CN	P	0.902	µg/l	5/10/2019 15:34:58	
CCV2	S	Total CN	P	248.1522	µg/l	5/10/2019 15:34:59	
CCB2	S	Total CN	P	-0.0321	µg/l	5/10/2019 15:35:00	
K2801-04	S	Total CN	P	0.256	µg/l	5/10/2019 15:35:01	
K2801-07	S	Total CN	P	0.1908	µg/l	5/10/2019 15:35:02	
CCV3	S	Total CN	P	250.473	µg/l	5/10/2019 15:35:03	
CCB3	S	Total CN	P	0.3298	µg/l	5/10/2019 15:35:04	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/10/2019 15:12


Test Total CN

Accepted 5/10/2019 12:09

Factor 995.7
Bias 0.004

Coeff. of det. 0.999967

Errors

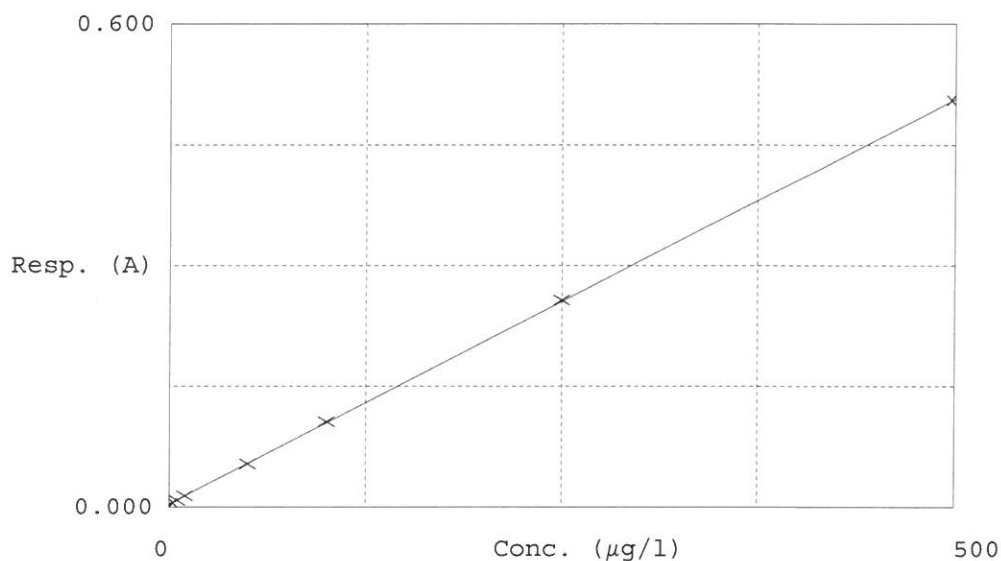

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.2793	0.0000	
2	5.0PPBCN	0.009	4.3408	5.0000	
3	10PPBCN	0.014	9.6349	10.0000	
4	50PPBCN	0.054	49.3677	50.0000	
5	100PPBCN	0.106	101.2120	100.0000	
6	250PPBCN	0.257	251.7782	250.0000	
7	500PPBCN	0.505	498.9456	500.0000	