

LB102716


7470A

INSTRUMENT ID: CU1

Linear

 μ Abs.:

44325

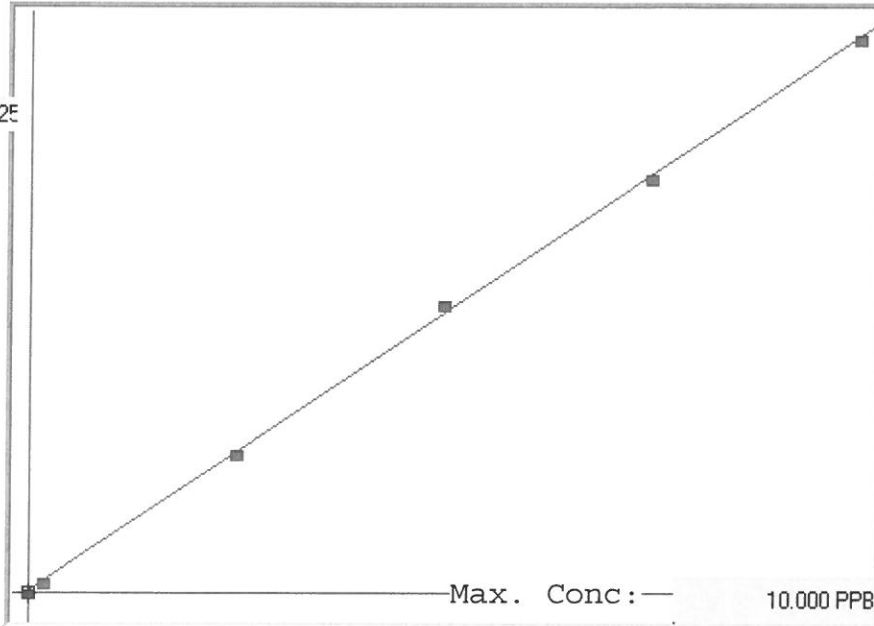

A= 0.0000e+000

B= 2.2524e-004

C= -3.2379e-002

Rho= 0.9997948

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.018	-0.018	64	0.000	64				
0.2	0.200	0.174	-0.026	915	0.0 %	915				
2.5	2.500	2.465	-0.035	11087	0.0 %	11087				
5.0	5.000	5.166	0.166	23078	0.0 %	23078				
7.5	7.500	7.462	-0.038	33272	0.0 %	33272				
10.0	10.000	9.952	-0.048	44325	0.0 %	44325				

LB102716 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 13 May 2019 17:06:12

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	64	-	0.0000	7470A	PPB	13 May 2019 17:07:10	S	Std
0.2 - 1	50-2	915	-	0.2000	7470A	PPB	13 May 2019 17:09:18	S	Std
2.5 - 1	52-5	11087	-	2.5000	7470A	PPB	13 May 2019 17:11:26	S	Std
5.0 - 1	55-0	23078	-	5.0000	7470A	PPB	13 May 2019 17:13:34	S	Std
7.5 - 1	57-5	33272	-	7.5000	7470A	PPB	13 May 2019 17:15:41	S	Std
10.0 - 1	510-0	44325	-	10.0000	7470A	PPB	13 May 2019 17:17:48	S	Std
ICV40 - 1	ICV40	16758	3.7423	-	7470A	PPB	13 May 2019 17:20:41	U	SMPL
ICB40 - 1	ICB40	-2	-0.0328	-	7470A	PPB	13 May 2019 17:22:47	U	SMPL
CCV05 - 1	CCV05	23224	5.1987	-	7470A	PPB	13 May 2019 17:24:52	U	SMPL
CCB05 - 1	CCB05	-12	-0.0351	-	7470A	PPB	13 May 2019 17:26:59	U	SMPL
CRA - 1	CRA	908	0.1721	-	7470A	PPB	13 May 2019 17:29:05	U	SMPL
HighStd - 1	HighStd	44969	10.0966	-	7470A	PPB	13 May 2019 17:31:11	U	SMPL
ChkStd - 1	ChkStd	31290	7.0155	-	7470A	PPB	13 May 2019 17:33:17	U	SMPL
PB119692BL - 1	PBW	-57	-0.0452	-	7470A	PPB	13 May 2019 17:35:24	U	SMPL
PB119692BS - 1	LCSW	17572	3.9256	-	7470A	PPB	13 May 2019 17:37:31	U	SMPL
K2795-02 - 1	TRUCK-803	6	-0.0310	-	7470A	PPB	13 May 2019 17:39:38	U	SMPL
K2795-02DUP - 1	TRUCK-803DUP	25	-0.0267	-	7470A	PPB	13 May 2019 17:41:46	U	SMPL
K2795-02MS - 1	TRUCK-803MS	17596	3.9310	-	7470A	PPB	13 May 2019 17:43:54	U	SMPL
K2795-02MSD - 1	TRUCK-803MSD	17169	3.8348	-	7470A	PPB	13 May 2019 17:46:02	U	SMPL
PB119692TB - 1	PB119671TB	-64	-0.0468	-	7470A	PPB	13 May 2019 17:48:08	U	SMPL
CCV06 - 1	CCV06	23042	5.1577	-	7470A	PPB	13 May 2019 17:50:14	U	SMPL
CCB06 - 1	CCB06	313	0.0381	-	7470A	PPB	13 May 2019 17:52:20	U	SMPL
K2795-02LX5 - 1		110	-0.0076	-	7470A	PPB	13 May 2019 17:54:26	U	SMPL
K2795-02A - 1		17221	3.8466	-	7470A	PPB	13 May 2019 17:56:32	U	SMPL
CCV07 - 1	CCV07	23157	5.1836	-	7470A	PPB	13 May 2019 17:58:39	U	SMPL
CCB07 - 1	CCB07	-54	-0.0445	-	7470A	PPB	13 May 2019 18:00:45	U	SMPL