

LB102721


245.1

INSTRUMENT ID: CU1

Linear

 μ Abs.:

43190

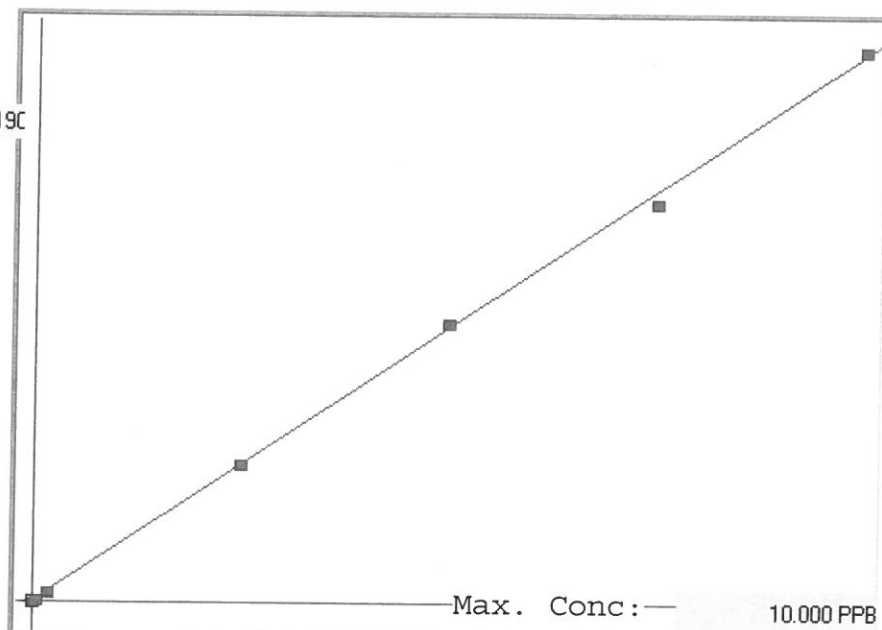

A= 0.0000e+000

B= 2.3369e-004

C= -9.0524e-003

Rho= 0.9997079

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.006	-0.006	13	0.000	13				
0.05	0.050	0.052	0.002	260	0.0 %	260				
0.2	0.200	0.188	-0.012	843	0.0 %	843				
2.5	2.500	2.527	0.027	10851	0.0 %	10851				
5.0	5.000	5.101	0.101	21868	0.0 %	21868				
7.5	7.500	7.305	-0.195	31297	0.0 %	31297				
10.0	10.000	10.084	0.084	43190	0.0 %	43190				

LB102721 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 14 May 2019 10:03:40

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	13	-	0.0000	245.1	PPB	14 May 2019 10:06:00	S	Std
0.05 - 1	50.05	260	-	0.0500	245.1	PPB	14 May 2019 10:08:18	S	Std
0.2 - 1	50.2	843	-	0.2000	245.1	PPB	14 May 2019 10:10:36	S	Std
2.5 - 1	52.5	10851	-	2.5000	245.1	PPB	14 May 2019 10:12:53	S	Std
5.0 - 1	55.0	21868	-	5.0000	245.1	PPB	14 May 2019 10:15:10	S	Std
7.5 - 1	57.5	31297	-	7.5000	245.1	PPB	14 May 2019 10:17:26	S	Std
10.0 - 1	510.0	43190	-	10.0000	245.1	PPB	14 May 2019 10:19:42	S	Std
ICV41 - 1	ICV41	17482	4.0763	-245.1		PPB	14 May 2019 10:43:20	U	SMPL
ICB41 - 1	ICB41	-33	-0.0168	-245.1		PPB	14 May 2019 10:45:34	U	SMPL
CCV08 - 1	CCV08	22351	5.2141	-245.1		PPB	14 May 2019 10:47:50	U	SMPL
CCB08 - 1	CCB08	67	0.0066	-245.1		PPB	14 May 2019 10:50:05	U	SMPL
CRA - 1	CRA	263	0.0524	-245.1		PPB	14 May 2019 10:52:20	U	SMPL
HighStd - 1	HighStd	45494	10.6223	-245.1		PPB	14 May 2019 10:54:35	U	SMPL
ChkStd - 1	ChkStd	30533	7.1261	-245.1		PPB	14 May 2019 10:56:51	U	SMPL
PB119711BL - 1	PBW	-92	-0.0306	-245.1		PPB	14 May 2019 10:59:08	U	SMPL
PB119711BS - 1	LCSW	17090	3.9846	-245.1		PPB	14 May 2019 11:01:25	U	SMPL
K2818-01 - 1	050919-ESLT-F-D-B	-18	-0.0133	-245.1		PPB	14 May 2019 11:03:42	U	SMPL
K2818-01DUP - 1	050919-ESLT-F-D-BDUP	13	-0.0060	-245.1		PPB	14 May 2019 11:05:59	U	SMPL
K2818-01MS - 1	050919-ESLT-F-D-BMS	17711	4.1298	-245.1		PPB	14 May 2019 11:08:16	U	SMPL
K2818-01MSD - 1	050919-ESLT-F-D-BMSD	17677	4.1218	-245.1		PPB	14 May 2019 11:10:33	U	SMPL
K2818-02 - 1	050919-ESLT-F-D-M	-57	-0.0224	-245.1		PPB	14 May 2019 11:12:49	U	SMPL
CCV09 - 1	CCV09	23157	5.4024	-245.1		PPB	14 May 2019 11:15:05	U	SMPL
CCB09 - 1	CCB09	-42	-0.0189	-245.1		PPB	14 May 2019 11:17:21	U	SMPL
K2818-03 - 1	050919-ESLT-F-D-S	36	-0.0006	-245.1		PPB	14 May 2019 11:19:37	U	SMPL
K2818-04 - 1	050919-ESLT-F-U-B	21	-0.0041	-245.1		PPB	14 May 2019 11:21:53	U	SMPL
K2818-05 - 1	050919-ESLT-F-U-M	16	-0.0053	-245.1		PPB	14 May 2019 11:24:08	U	SMPL
K2818-06 - 1	050919-ESLT-F-U-S	28	-0.0025	-245.1		PPB	14 May 2019 11:26:24	U	SMPL
K2818-01LX5 - 1		23	-0.0037	-245.1		PPB	14 May 2019 11:28:40	U	SMPL
K2818-01A - 1		17402	4.0576	-245.1		PPB	14 May 2019 11:30:57	U	SMPL
CCV10 - 1	CCV10	20477	4.7761	-245.1		PPB	14 May 2019 11:33:14	U	SMPL
CCB10 - 1	CCB10	-25	-0.0149	-245.1		PPB	14 May 2019 11:38:23	U	SMPL