

LB102794


7470A

INSTRUMENT ID : CU1

Linear

 μ Abs.:

43729

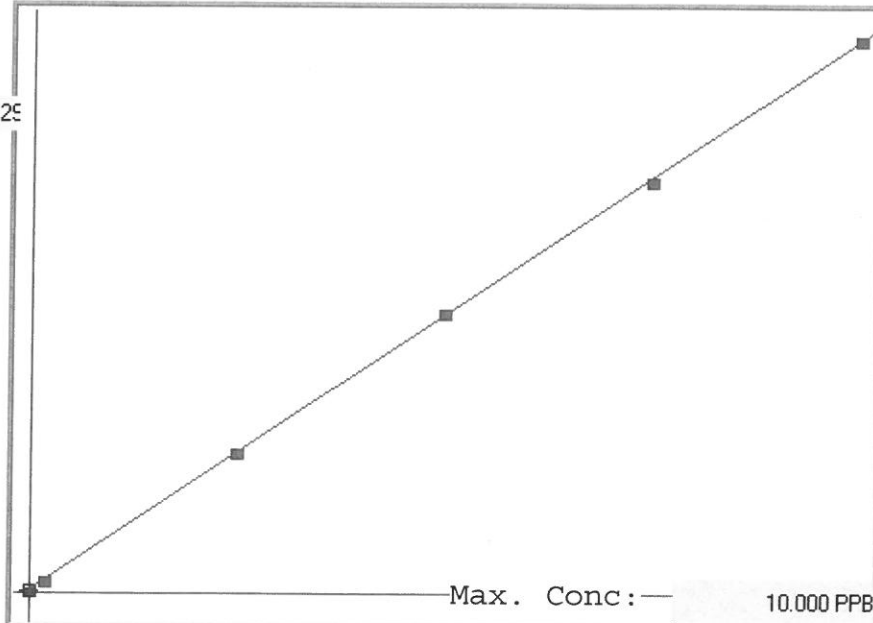

A= 0.0000e+000

B= 2.3000e-004

C= -5.4793e-002

Rho= 0.9999662

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.002	0.002	245	0.000	245				
0.2	0.200	0.188	-0.012	1055	0.0 %	1055				
2.5	2.500	2.488	-0.012	11055	0.0 %	11055				
5.0	5.000	5.060	0.060	22239	0.0 %	22239				
7.5	7.500	7.460	-0.040	32673	0.0 %	32673				
10.0	10.000	10.003	0.003	43729	0.0 %	43729				

LB102794 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 16 May 2019 14:39:04

Sample ID	Extended ID	µ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	245	-	0.0000	7470A	PPB	16 May 2019 14:42:43	S	Std
0.2 - 1	50.2	1055	-	0.2000	7470A	PPB	16 May 2019 14:44:56	S	Std
2.5 - 1	52.5	11055	-	2.5000	7470A	PPB	16 May 2019 14:47:04	S	Std
5.0 - 1	54.0	22239	-	5.0000	7470A	PPB	16 May 2019 14:49:12	S	Std
7.5 - 1	57.5	32673	-	7.5000	7470A	PPB	16 May 2019 14:51:19	S	Std
10.0 - 1	510.0	43729	-	10.0000	7470A	PPB	16 May 2019 14:56:13	S	Std
ICV45 - 1	ICV45	17162	3.8924	-	7470A	PPB	16 May 2019 14:58:53	U	SMPL
ICB45 - 1	ICB45	152	-0.0198	-	7470A	PPB	16 May 2019 15:00:59	U	SMPL
CCV21 - 1	CCV21	22499	5.1199	-	7470A	PPB	16 May 2019 15:03:05	U	SMPL
CCB21 - 1	CCB21	154	-0.0194	-	7470A	PPB	16 May 2019 15:05:11	U	SMPL
CRA - 1	CRA	1054	0.1876	-	7470A	PPB	16 May 2019 15:07:16	U	SMPL
HighStd - 1	HighStd	44439	10.1660	-	7470A	PPB	16 May 2019 15:09:22	U	SMPL
ChkStd - 1	ChkStd	30620	6.9877	-	7470A	PPB	16 May 2019 15:11:29	U	SMPL
PB119795BL - 1	PBW	291	0.0121	-	7470A	PPB	16 May 2019 15:13:37	U	SMPL
PB119795BS - 1	LCSW	18130	4.1151	-	7470A	PPB	16 May 2019 15:15:44	U	SMPL
K2637-02 - 1	HR-06-051519-A	887	0.1492	-	7470A	PPB	16 May 2019 15:17:51	U	SMPL
K2637-02DUP - 1	HR-06-051519-ADUP	1080	0.1936	-	7470A	PPB	16 May 2019 15:19:59	U	SMPL
K2637-02MS - 1	HR-06-051519-AMS	18615	4.2266	-	7470A	PPB	16 May 2019 15:22:07	U	SMPL
K2637-02MSD - 1	HR-06-051519-AMSD	18753	4.2583	-	7470A	PPB	16 May 2019 15:24:15	U	SMPL
K2637-04 - 1	HR-06-051519-B	472	0.0538	-	7470A	PPB	16 May 2019 15:26:21	U	SMPL
CCV22 - 1	CCV22	22581	5.1388	-	7470A	PPB	16 May 2019 15:28:27	U	SMPL
CCB22 - 1	CCB22	180	-0.0134	-	7470A	PPB	16 May 2019 15:30:34	U	SMPL
K2644-02 - 1	EO-01-051519-A	379	0.0324	-	7470A	PPB	16 May 2019 15:32:40	U	SMPL
K2644-04 - 1	EO-01-051519-B	418	0.0413	-	7470A	PPB	16 May 2019 15:34:46	U	SMPL
K2865-04 - 1	TP-21-S	480	0.0556	-	7470A	PPB	16 May 2019 15:36:53	U	SMPL
K2865-08 - 1	TP-22-S	476	0.0547	-	7470A	PPB	16 May 2019 15:38:59	U	SMPL
K2865-12 - 1	TP-22-D	411	0.0397	-	7470A	PPB	16 May 2019 15:41:06	U	SMPL
K2866-03 - 1	RO-COMP-1	494	0.0588	-	7470A	PPB	16 May 2019 15:43:13	U	SMPL
K2866-06 - 1	RO-COMP-2	495	0.0591	-	7470A	PPB	16 May 2019 15:45:21	U	SMPL
K2866-09 - 1	RO-COMP-3	439	0.0462	-	7470A	PPB	16 May 2019 15:47:29	U	SMPL
K2870-01 - 1	OIL-DRUM	432	0.0446	-	7470A	PPB	16 May 2019 15:49:37	U	SMPL
K2870-03 - 1	OIL-DEBRIS	400	0.0372	-	7470A	PPB	16 May 2019 15:51:43	U	SMPL
CCV23 - 1	CCV23	22098	5.0277	-	7470A	PPB	16 May 2019 15:53:50	U	SMPL
CCB23 - 1	CCB23	173	-0.0150	-	7470A	PPB	16 May 2019 15:55:57	U	SMPL
PB119796BL - 1	PBW	345	0.0246	-	7470A	PPB	16 May 2019 15:58:03	U	SMPL
PB119796BS - 1	LCSW	17689	4.0136	-	7470A	PPB	16 May 2019 16:00:09	U	SMPL
K2838-07 - 1	FEQC-FB-051419	309	0.0163	-	7470A	PPB	16 May 2019 16:02:16	U	SMPL
K2852-01 - 1	TP-GROUNDWATER	4539	0.9892	-	7470A	PPB	16 May 2019 16:04:23	U	SMPL
K2861-02 - 1	TT-001-IDWGW-20190514	797	0.1285	-	7470A	PPB	16 May 2019 16:06:29	U	SMPL
K2861-02DUP - 1	TT-001-IDWGW-20190514DUP	785	0.1258	-	7470A	PPB	16 May 2019 16:08:37	U	SMPL
K2861-02MS - 1	TT-001-IDWGW-20190514MS	17290	3.9219	-	7470A	PPB	16 May 2019 16:10:44	U	SMPL
K2861-02MSD - 1	TT-001-IDWGW-20190514MSD	18093	4.1065	-	7470A	PPB	16 May 2019 16:12:52	U	SMPL
PB119799BL - 1	PBW	301	0.0144	-	7470A	PPB	16 May 2019 16:15:00	U	SMPL
PB119799BS - 1	LCSW	16968	3.8478	-	7470A	PPB	16 May 2019 16:17:07	U	SMPL
CCV24 - 1	CCV24	21642	4.9228	-	7470A	PPB	16 May 2019 16:19:13	U	SMPL
CCB24 - 1	CCB24	158	-0.0185	-	7470A	PPB	16 May 2019 16:21:20	U	SMPL
K2852-02 - 1	TP-GROUNDWATER	281	0.0098	-	7470A	PPB	16 May 2019 16:23:26	U	SMPL
K2880-05 - 1	339	298	0.0137	-	7470A	PPB	16 May 2019 16:25:33	U	SMPL
K2880-05DUP - 1	339DUP	309	0.0163	-	7470A	PPB	16 May 2019 16:27:40	U	SMPL
K2880-05MS - 1	339MS	16189	3.6686	-	7470A	PPB	16 May 2019 16:29:46	U	SMPL
K2880-05MSD - 1	339MSD	15989	3.6226	-	7470A	PPB	16 May 2019 16:31:53	U	SMPL
PB119800BL - 1	PBW	155	-0.0191	-	7470A	PPB	16 May 2019 16:34:00	U	SMPL
PB119800BS - 1	LCSW	17044	3.8653	-	7470A	PPB	16 May 2019 16:36:08	U	SMPL
K2851-03 - 1	SOIL-COMP	628	0.0896	-	7470A	PPB	16 May 2019 16:38:15	U	SMPL
K2851-03DUP - 1	SOIL-COMPDUP	711	0.1087	-	7470A	PPB	16 May 2019 16:40:23	U	SMPL
K2851-03MS - 1	SOIL-COMPMS	16713	3.7891	-	7470A	PPB	16 May 2019 16:42:30	U	SMPL
CCV25 - 1	CCV25	21575	4.9074	-	7470A	PPB	16 May 2019 16:44:37	U	SMPL
CCB25 - 1	CCB25	159	-0.0182	-	7470A	PPB	16 May 2019 16:46:44	U	SMPL
K2851-03MSD - 1	SOIL-COMPMSD	16842	3.8188	-	7470A	PPB	16 May 2019 16:48:50	U	SMPL
PB119795TB - 1	PB119765TB	469	0.0531	-	7470A	PPB	16 May 2019 16:50:57	U	SMPL
PB119799TB - 1	PB119787TB	499	0.0600	-	7470A	PPB	16 May 2019 16:53:03	U	SMPL
PB119800TB - 1	PB119736TB	81	-0.0362	-	7470A	PPB	16 May 2019 16:55:10	U	SMPL
K2637-02LX5 - 1		257	0.0043	-	7470A	PPB	16 May 2019 16:57:17	U	SMPL
K2637-02A - 1		17543	3.9800	-	7470A	PPB	16 May 2019 16:59:24	U	SMPL
K2861-02LX5 - 1		217	-0.0049	-	7470A	PPB	16 May 2019 17:01:31	U	SMPL
K2861-02A - 1		18441	4.1866	-	7470A	PPB	16 May 2019 17:03:39	U	SMPL
K2880-05LX5 - 1		101	-0.0316	-	7470A	PPB	16 May 2019 17:05:47	U	SMPL
K2880-05A - 1		16479	3.7353	-	7470A	PPB	16 May 2019 17:07:54	U	SMPL
CCV26 - 1	CCV26	21667	4.9286	-	7470A	PPB	16 May 2019 17:10:03	U	SMPL
CCB26 - 1	CCB26	125	-0.0260	-	7470A	PPB	16 May 2019 17:12:11	U	SMPL
K2851-03LX5 - 1		201	-0.0086	-	7470A	PPB	16 May 2019 17:14:17	U	SMPL
K2851-03A - 1		16556	3.7530	-	7470A	PPB	16 May 2019 17:16:25	U	SMPL
CCV27 - 1	CCV27	20919	4.7565	-	7470A	PPB	16 May 2019 17:18:32	U	SMPL
CCB27 - 1	CCB27	170	-0.0157	-	7470A	PPB	16 May 2019 17:20:38	U	SMPL