


LB102832

245.1

INSTRUMENT ID: CV1

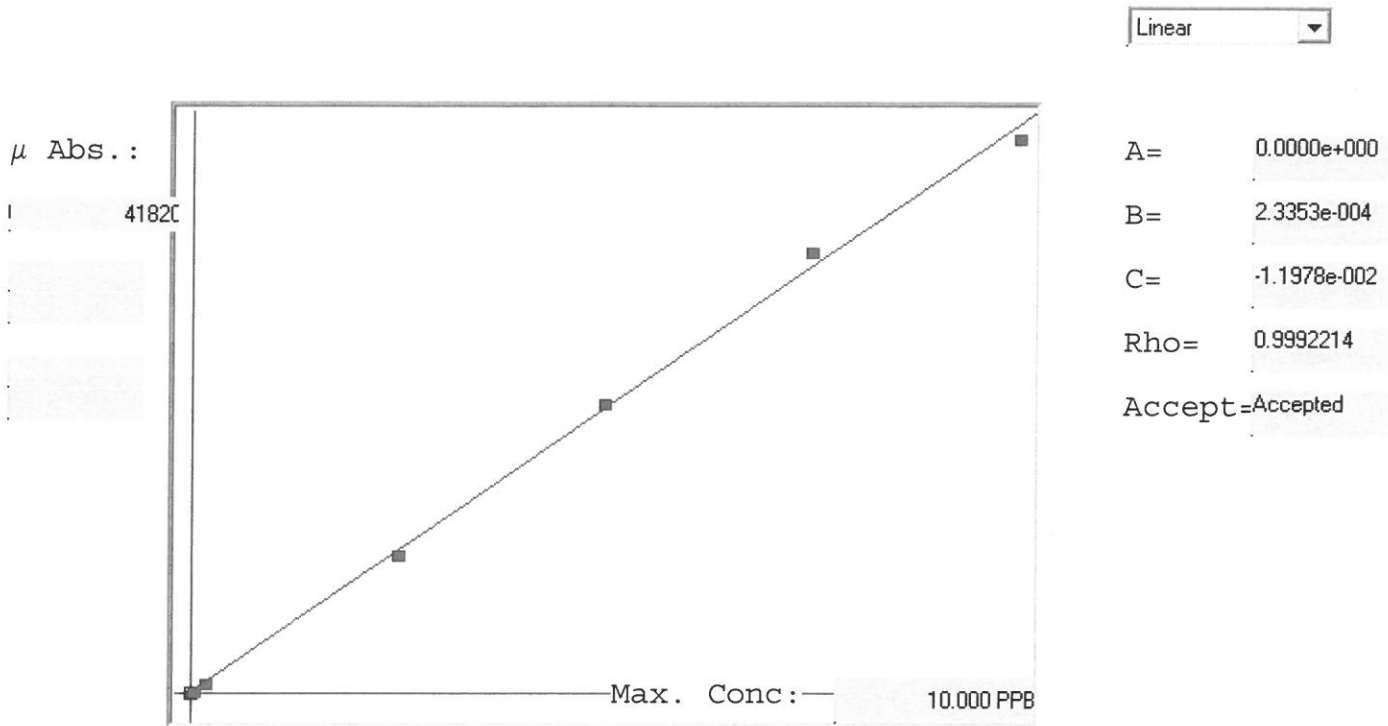

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.002	-0.002	42	0.000	42				
0.05	0.050	0.043	-0.007	235	0.0 %	235				
0.2	0.200	0.167	-0.033	767	0.0 %	767				
2.5	2.500	2.423	-0.077	10427	0.0 %	10427				
5.0	5.000	5.092	0.092	21855	0.0 %	21855				
7.5	7.500	7.773	0.273	33334	0.0 %	33334				
10.0	10.000	9.754	-0.246	41820	0.0 %	41820				

LB102832 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 17 May 2019 16:14:38

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	42	-	0.0000	245.1	PPB	17 May 2019 16:16:01	S	Std
0.05 - 1	50.05	235	-	0.0500	245.1	PPB	17 May 2019 16:18:18	S	Std
0.2 - 1	50.2	767	-	0.2000	245.1	PPB	17 May 2019 16:20:36	S	Std
2.5 - 1	52.5	10427	-	2.5000	245.1	PPB	17 May 2019 16:22:53	S	Std
5.0 - 1	55.0	21855	-	5.0000	245.1	PPB	17 May 2019 16:25:10	S	Std
7.5 - 1	57.5	33334	-	7.5000	245.1	PPB	17 May 2019 16:27:26	S	Std
10.0 - 1	510.0	41820	-	10.0000	245.1	PPB	17 May 2019 16:29:41	S	Std
ICV48 - 1	ICV48	16250	3.7830	-245.1		PPB	17 May 2019 16:33:50	U	SMPL
ICB48 - 1	ICB48	-27	-0.0183	-245.1		PPB	17 May 2019 16:36:05	U	SMPL
CCV39 - 1	CCV39	21803	5.0798	-245.1		PPB	17 May 2019 16:38:21	U	SMPL
CCB39 - 1	CCB39	-26	-0.0180	-245.1		PPB	17 May 2019 16:40:36	U	SMPL
CRA - 1	CRA	216	0.0385	-245.1		PPB	17 May 2019 16:42:51	U	SMPL
HighStd - 1	HighStd	41431	9.6636	-245.1		PPB	17 May 2019 16:45:07	U	SMPL
ChkStd - 1	ChkStd	29791	6.9453	-245.1		PPB	17 May 2019 16:47:23	U	SMPL
PB119842BL - 1	PBW	-60	-0.0260	-245.1		PPB	17 May 2019 16:49:39	U	SMPL
PB119842BS - 1	LCSW	15809	3.6800	-245.1		PPB	17 May 2019 16:51:56	U	SMPL
K2841-01 - 1	051019-LIFT-F-D-B	145	0.0219	-245.1		PPB	17 May 2019 16:58:25	U	SMPL
K2841-01DUP - 1	051019-LIFT-F-D-BDUP	148	0.0226	-245.1		PPB	17 May 2019 17:00:42	U	SMPL
K2841-01MS - 1	051019-LIFT-F-D-BMS	16058	3.7381	-245.1		PPB	17 May 2019 17:23:21	U	SMPL
K2841-01MSD - 1	051019-LIFT-F-D-BMSD	15724	3.6601	-245.1		PPB	17 May 2019 17:25:38	U	SMPL
K2841-02 - 1	051019-LIFT-F-D-M	55	0.0009	-245.1		PPB	17 May 2019 17:33:31	U	SMPL
CCV40 - 1	CCV40	21837	5.0877	-245.1		PPB	17 May 2019 17:35:46	U	SMPL
CCB40 - 1	CCB40	-83	-0.0314	-245.1		PPB	17 May 2019 17:38:02	U	SMPL
K2841-03 - 1	051019-LIFT-F-D-S	40	-0.0026	-245.1		PPB	17 May 2019 17:40:17	U	SMPL
K2841-04 - 1	051019-LIFT-F-U-B	-2	-0.0124	-245.1		PPB	17 May 2019 17:46:21	U	SMPL
K2841-05 - 1	051019-LIFT-F-U-M	26	-0.0059	-245.1		PPB	17 May 2019 17:48:36	U	SMPL
K2841-06 - 1	051019-LIFT-F-U-S	26	-0.0059	-245.1		PPB	17 May 2019 17:50:51	U	SMPL
K2842-02 - 1	051119-LIFT-F-D-B	21	-0.0071	-245.1		PPB	17 May 2019 17:53:08	U	SMPL
K2842-03 - 1	051119-LIFT-F-D-M	14	-0.0087	-245.1		PPB	17 May 2019 17:55:24	U	SMPL
K2842-04 - 1	051119-LIFT-F-D-S	4	-0.0110	-245.1		PPB	17 May 2019 17:57:41	U	SMPL
K2842-05 - 1	051119-LIFT-F-U-B	11	-0.0094	-245.1		PPB	17 May 2019 17:59:58	U	SMPL
K2842-06 - 1	051119-LIFT-F-U-M	11	-0.0094	-245.1		PPB	17 May 2019 18:02:15	U	SMPL
K2842-07 - 1	051119-LIFT-F-U-S	5	-0.0108	-245.1		PPB	17 May 2019 18:04:31	U	SMPL
CCV41 - 1	CCV41	13	-0.0089	-245.1		PPB	17 May 2019 18:06:47	U	SMPL
CCB41 - 1	CCB41	12	-0.0092	-245.1		PPB	17 May 2019 18:09:02	U	SMPL
CCV41 - 1	CCV41	21279	4.9574	-245.1		PPB	17 May 2019 18:20:14	U	SMPL
CCB41 - 1	CCB41	-57	-0.0253	-245.1		PPB	17 May 2019 18:22:29	U	SMPL
K2844-03 - 1	HP-627	440	0.0908	-245.1		PPB	17 May 2019 18:27:01	U	SMPL
K2844-04 - 1	HP-627-X	401	0.0817	-245.1		PPB	17 May 2019 18:29:16	U	SMPL
K2844-07 - 1	HP-640	319	0.0625	-245.1		PPB	17 May 2019 18:31:33	U	SMPL
K2841-01LX5 - 1		15	-0.0085	-245.1		PPB	17 May 2019 18:33:49	U	SMPL
K2841-01A - 1		16876	3.9292	-245.1		PPB	17 May 2019 18:36:05	U	SMPL
k2844-01 - 1		64	0.0030	-245.1		PPB	17 May 2019 18:38:22	U	SMPL
CCV42 - 1	CCV42	21253	4.9513	-245.1		PPB	17 May 2019 18:40:40	U	SMPL
CCB42 - 1	CCB42	-59	-0.0258	-245.1		PPB	17 May 2019 18:42:57	U	SMPL