

LB102936


7471B

INSTRUMENT ID: CU1

Linear

 μ Abs.:

62651

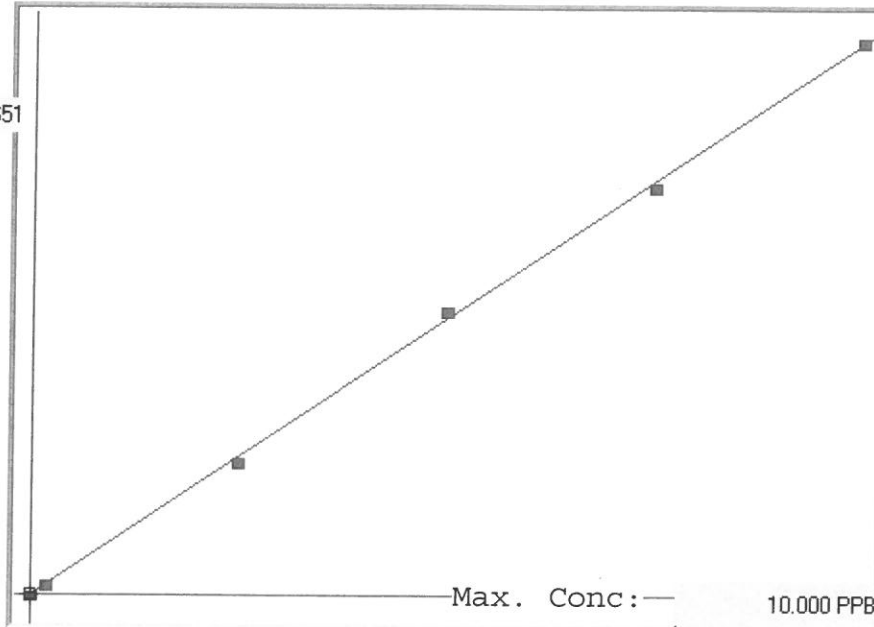

A= 0.0000e+000

B= 1.5992e-004

C= 5.6614e-003

Rho= 0.9997335

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.014	0.014	51	0.000	51				
0.2	0.200	0.211	0.011	1284	0.0 %	1284				
2.5	2.500	2.409	-0.091	15031	0.0 %	15031				
5.0	5.000	5.150	0.150	32167	0.0 %	32167				
7.5	7.500	7.391	-0.109	46179	0.0 %	46179				
10.0	10.000	10.025	0.025	62651	0.0 %	62651				

LB102936 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 23 May 2019 09:48:05

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	51	-	0.00007471B	PPB		23 May 2019 09:51:07	S	Std
0.2 - 1	50-2	1284	-	0.20007471B	PPB		23 May 2019 09:53:25	S	Std
2.5 - 1	52-5	15031	-	2.50007471B	PPB		23 May 2019 09:55:43	S	Std
5.0 - 1	55-0	32167	-	5.00007471B	PPB		23 May 2019 09:58:00	S	Std
7.5 - 1	57-5	46179	-	7.50007471B	PPB		23 May 2019 10:00:17	S	Std
10.0 - 1	510-0	62651	-	10.00007471B	PPB		23 May 2019 10:02:34	S	Std
ICV57 - 1	ICV57	24739	3.9620	-7471B	PPB		23 May 2019 10:05:52	U	SMPL
ICB57 - 1	ICB57	-20	0.0025	-7471B	PPB		23 May 2019 10:08:07	U	SMPL
CCV79 - 1	CCV79	31897	5.1067	-7471B	PPB		23 May 2019 10:10:23	U	SMPL
CCB79 - 1	CCB79	-19	0.0026	-7471B	PPB		23 May 2019 10:12:38	U	SMPL
CRA - 1	CRA	1246	0.2049	-7471B	PPB		23 May 2019 10:14:54	U	SMPL
HighStd - 1	HighStd	61741	9.8795	-7471B	PPB		23 May 2019 10:17:10	U	SMPL
ChkStd - 1	ChkStd	43011	6.8841	-7471B	PPB		23 May 2019 10:19:26	U	SMPL
PB119980BL - 1	PBS	-104	-0.0110	-7471B	PPB		23 May 2019 10:21:44	U	SMPL
PB119980BS - 1	LCSS	22215	3.5584	-7471B	PPB		23 May 2019 10:24:02	U	SMPL
K2642-05 - 1	OK-01-052119	1647	0.2691	-7471B	PPB		23 May 2019 10:26:18	U	SMPL
K2642-05DUP - 1	OK-01-052119DUP	1645	0.2687	-7471B	PPB		23 May 2019 10:28:36	U	SMPL
K2642-05MS - 1	OK-01-052119MS	24244	3.8828	-7471B	PPB		23 May 2019 10:30:53	U	SMPL
K2642-05MSD - 1	OK-01-052119MSD	24427	3.9121	-7471B	PPB		23 May 2019 10:33:10	U	SMPL
K2753-01 - 1	CONCRETE-1	244	0.0447	-7471B	PPB		23 May 2019 10:35:27	U	SMPL
CCV80 - 1	CCV80	32523	5.2069	-7471B	PPB		23 May 2019 10:37:43	U	SMPL
CCB80 - 1	CCB80	-43	-0.0012	-7471B	PPB		23 May 2019 10:39:59	U	SMPL
K2753-02 - 1	CONCRETE-2	376	0.0658	-7471B	PPB		23 May 2019 10:42:15	U	SMPL
K2753-03 - 1	CONCRETE-3	1786	0.2913	-7471B	PPB		23 May 2019 10:44:31	U	SMPL
K2753-04 - 1	CONCRETE-4	1944	0.3166	-7471B	PPB		23 May 2019 10:46:47	U	SMPL
K2753-05 - 1	CONCRETE-5	87	0.0196	-7471B	PPB		23 May 2019 10:49:03	U	SMPL
K2970-03 - 1	TP-11-S	25135	4.0253	-7471B	PPB		23 May 2019 10:51:19	U	SMPL
K2970-07 - 1	TP-11-D	22879	3.6645	-7471B	PPB		23 May 2019 10:53:36	U	SMPL
K2970-15 - 1	TP-9-S	6407	1.0303	-7471B	PPB		23 May 2019 10:55:54	U	SMPL
K2971-12 - 1	SUP-2A-C-1-052019	2670	0.4327	-7471B	PPB		23 May 2019 10:58:12	U	SMPL
K2971-13 - 1	SUP-2A-C-2-052019	898	0.1493	-7471B	PPB		23 May 2019 11:00:30	U	SMPL
K2971-14 - 1	SUP-2A-C-3-052019	1404	0.2302	-7471B	PPB		23 May 2019 11:02:46	U	SMPL
CCV81 - 1	CCV81	32046	5.1306	-7471B	PPB		23 May 2019 11:05:02	U	SMPL
CCB81 - 1	CCB81	-18	0.0028	-7471B	PPB		23 May 2019 11:07:18	U	SMPL
K2971-15 - 1	SUP-2A-C-4-052019	1313	0.2156	-7471B	PPB		23 May 2019 11:09:35	U	SMPL
K2971-17 - 1	SUP-2C-C-1-052019	1622	0.2651	-7471B	PPB		23 May 2019 11:11:51	U	SMPL
K2978-01 - 1	RO-SOIL	358	0.0629	-7471B	PPB		23 May 2019 11:14:07	U	SMPL
K2978-06 - 1	TP-SOIL	10464	1.6791	-7471B	PPB		23 May 2019 11:16:24	U	SMPL
K2986-01 - 1	FESB-19(6.5-7)	2613	0.4235	-7471B	PPB		23 May 2019 11:18:40	U	SMPL
K2986-02 - 1	FESB-21(4.5-5)	1013	0.1677	-7471B	PPB		23 May 2019 11:20:57	U	SMPL
K2986-03 - 1	FEQC-052119	1500	0.2455	-7471B	PPB		23 May 2019 11:23:14	U	SMPL
PB119993BL - 1	PBS	37	0.0116	-7471B	PPB		23 May 2019 11:25:31	U	SMPL
PB119993BS - 1	LCSS	22901	3.6681	-7471B	PPB		23 May 2019 11:27:49	U	SMPL
K2647-11 - 1	SU-03-052219-A	2094	0.3405	-7471B	PPB		23 May 2019 11:30:05	U	SMPL
CCV82 - 1	CCV82	31559	5.0527	-7471B	PPB		23 May 2019 11:32:21	U	SMPL
CCB82 - 1	CCB82	-26	0.0015	-7471B	PPB		23 May 2019 11:34:36	U	SMPL
K2647-13 - 1	SU-03-052219-B	6880	1.1059	-7471B	PPB		23 May 2019 11:36:53	U	SMPL
K2993-16 - 1	COMP-1	4611	0.7431	-7471B	PPB		23 May 2019 11:39:09	U	SMPL
K2993-17 - 1	COMP-2	1387	0.2275	-7471B	PPB		23 May 2019 11:41:25	U	SMPL
K2993-18 - 1	COMP-3	1368	0.2244	-7471B	PPB		23 May 2019 11:43:41	U	SMPL
K2994-03 - 1	TP-8-S	14607	2.3417	-7471B	PPB		23 May 2019 11:45:57	U	SMPL
K2994-07 - 1	TP-8-D	4799	0.7731	-7471B	PPB		23 May 2019 11:48:14	U	SMPL
K2994-15 - 1	TP-6-S	27431	4.3925	-7471B	PPB		23 May 2019 11:50:31	U	SMPL
K2998-01 - 1	EWING-SP	8089	1.2993	-7471B	PPB		23 May 2019 11:52:49	U	SMPL
K3002-01 - 1	COMP-Z1-20190418	19023	3.0479	-7471B	PPB		23 May 2019 11:55:07	U	SMPL
K3002-02 - 1	COMP-Z2-20190419	22165	3.5504	-7471B	PPB		23 May 2019 11:57:23	U	SMPL
CCV83 - 1	CCV83	30307	4.8525	-7471B	PPB		23 May 2019 11:59:39	U	SMPL
CCB83 - 1	CCB83	-37	-0.0003	-7471B	PPB		23 May 2019 12:01:56	U	SMPL
K3002-03 - 1	COMP-Z3-20190420	27041	4.3302	-7471B	PPB		23 May 2019 12:04:14	U	SMPL
K3004-01 - 1	CHRT-26835	1854	0.3022	-7471B	PPB		23 May 2019 12:06:30	U	SMPL
K3008-01 - 1	COMP-19	11424	1.8326	-7471B	PPB		23 May 2019 12:08:47	U	SMPL
K3008-03 - 1	COMP-20	15527	2.4888	-7471B	PPB		23 May 2019 12:11:03	U	SMPL
K3008-05 - 1	COMP-21	20418	3.2710	-7471B	PPB		23 May 2019 12:13:20	U	SMPL
K3010-01 - 1	FESB-20(2.5-3)	377	0.0660	-7471B	PPB		23 May 2019 12:15:36	U	SMPL
K3010-02 - 1	FESB-23(3-3.5)	1591	0.2601	-7471B	PPB		23 May 2019 12:17:54	U	SMPL
K3010-02DUP - 1	FESB-23(3-3.5)DUP	1545	0.2527	-7471B	PPB		23 May 2019 12:20:11	U	SMPL
K3010-03 - 1	FESB-22(1.5-2)	1006	0.1665	-7471B	PPB		23 May 2019 12:22:28	U	SMPL
K3010-04 - 1	k3010-02MS	25446	4.0751	-7471B	PPB		23 May 2019 12:24:44	U	SMPL
CCV84 - 1	CCV84	31335	5.0169	-7471B	PPB		23 May 2019 12:27:00	U	SMPL
CCB84 - 1	CCB84	-17	0.0029	-7471B	PPB		23 May 2019 12:29:17	U	SMPL
K3010-05 - 1	k3010-02MSD	26126	4.1838	-7471B	PPB		23 May 2019 12:31:34	U	SMPL
K2642-05LX5 - 1		281	0.0506	-7471B	PPB		23 May 2019 12:33:50	U	SMPL
K2642-05A - 1		24876	3.9839	-7471B	PPB		23 May 2019 12:36:08	U	SMPL
K3010-02LX5 - 1		263	0.0477	-7471B	PPB		23 May 2019 12:38:24	U	SMPL
K3010-02A - 1		26532	4.2487	-7471B	PPB		23 May 2019 12:40:41	U	SMPL
CCV85 - 1	CCV85	32570	5.2144	-7471B	PPB		23 May 2019 12:42:58	U	SMPL
CCB85 - 1	CCB85	-16	0.0031	-7471B	PPB		23 May 2019 12:45:15	U	SMPL