


LB102992

INSTRUMENT ID : CV1

7470A

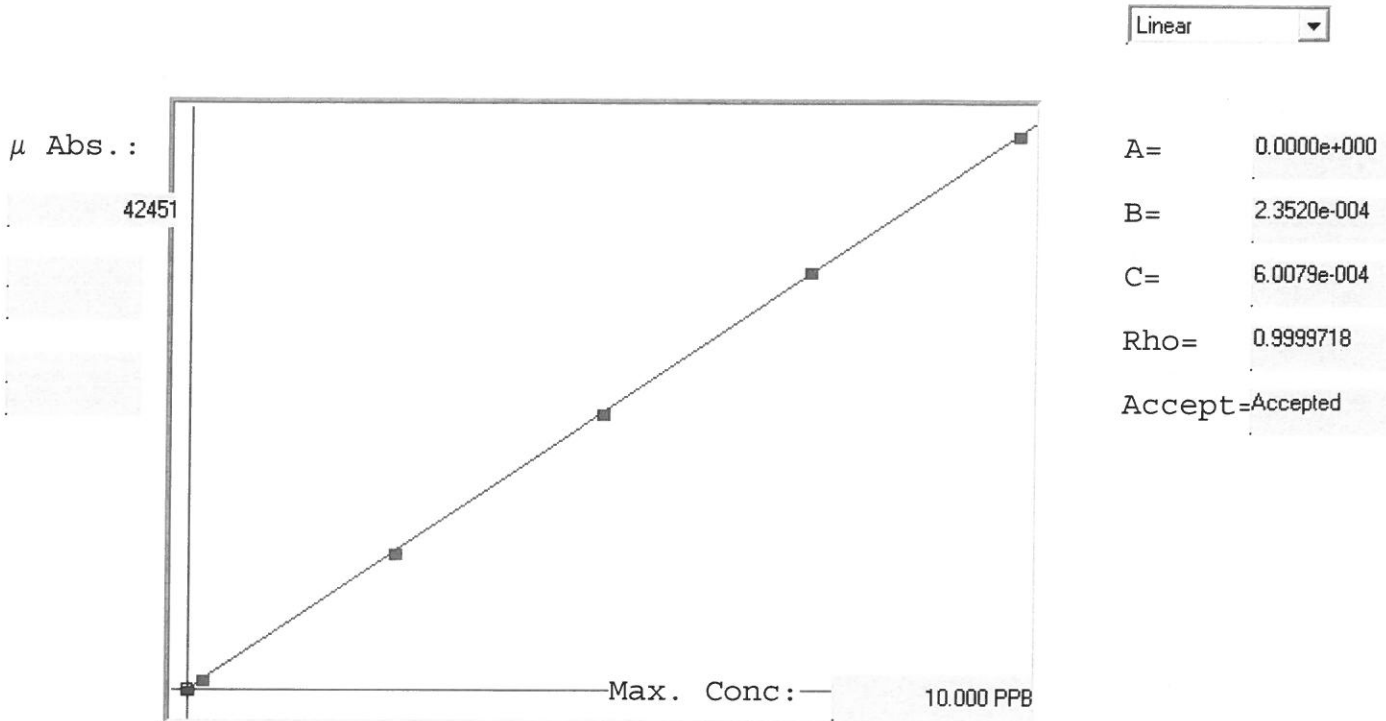

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.035	0.035	146	0.000	146				
0.2	0.200	0.187	-0.013	792	0.0 %	792				
2.5	2.500	2.469	-0.031	10493	0.0 %	10493				
5.0	5.000	4.983	-0.017	21185	0.0 %	21185				
7.5	7.500	7.541	0.041	32062	0.0 %	32062				
10.0	10.000	9.985	-0.015	42451	0.0 %	42451				

LB102992 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 24 May 2019 15:04:39

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	80.0	146	-	0.0000	7470A	PPB	24 May 2019 15:10:08	S	Std
0.2 - 1	80.2	792	-	0.2000	7470A	PPB	24 May 2019 15:12:16	S	Std
2.5 - 1	82.5	10493	-	2.5000	7470A	PPB	24 May 2019 15:14:24	S	Std
5.0 - 1	85.0	21185	-	5.0000	7470A	PPB	24 May 2019 15:16:32	S	Std
7.5 - 1	87.5	32062	-	7.5000	7470A	PPB	24 May 2019 15:18:39	S	Std
10.0 - 1	810.0	42451	-	10.0000	7470A	PPB	24 May 2019 15:20:46	S	Std
ICV61 - 1	ICV61	17363	4.0843	-	7470A	PPB	24 May 2019 15:24:55	U	SMPL
ICB61 - 1	ICB61	41	0.0102	-	7470A	PPB	24 May 2019 15:27:01	U	SMPL
CCV99 - 1	CCV99	21046	4.9506	-	7470A	PPB	24 May 2019 15:29:07	U	SMPL
CCB99 - 1	CCB99	-65	-0.0147	-	7470A	PPB	24 May 2019 15:31:13	U	SMPL
CRA - 1	CRA	793	0.1871	-	7470A	PPB	24 May 2019 15:33:18	U	SMPL
HighStd - 1	HighStd	42446	9.9838	-	7470A	PPB	24 May 2019 15:35:24	U	SMPL
ChkStd - 1	ChkStd	29736	6.9944	-	7470A	PPB	24 May 2019 15:37:31	U	SMPL
PB120061BL - 1	PBW	8	0.0025	-	7470A	PPB	24 May 2019 15:39:39	U	SMPL
PB120061BS - 1	LCSW	17605	4.1412	-	7470A	PPB	24 May 2019 15:41:47	U	SMPL
K2647-12 - 1	SU-03-052219-A	75	0.0182	-	7470A	PPB	24 May 2019 15:43:54	U	SMPL
K2647-12DUP - 1	SU-03-052219-ADUP	155	0.0371	-	7470A	PPB	24 May 2019 15:46:02	U	SMPL
K2647-12MS - 1	SU-03-052219-AMS	17787	4.1840	-	7470A	PPB	24 May 2019 15:48:10	U	SMPL
K2647-12MSD - 1	SU-03-052219-AMSD	18076	4.2520	-	7470A	PPB	24 May 2019 15:50:17	U	SMPL
K2647-14 - 1	SU-03-052219-B	-8	-0.0013	-	7470A	PPB	24 May 2019 15:52:24	U	SMPL
CCV01 - 1	CCV01	21256	4.9999	-	7470A	PPB	24 May 2019 15:54:30	U	SMPL
CCB01 - 1	CCB01	-67	-0.0152	-	7470A	PPB	24 May 2019 15:56:37	U	SMPL
K2994-04 - 1	TP-8-S	107	0.0258	-	7470A	PPB	24 May 2019 15:58:43	U	SMPL
K2994-08 - 1	TP-8-D	111	0.0267	-	7470A	PPB	24 May 2019 16:00:50	U	SMPL
K2994-16 - 1	TP-6-S	109	0.0262	-	7470A	PPB	24 May 2019 16:02:57	U	SMPL
K2997-01 - 1	DPC-81626-FB-01	65	0.0159	-	7470A	PPB	24 May 2019 16:05:03	U	SMPL
K2997-02 - 1	DPC-81626-FB-02	98	0.0237	-	7470A	PPB	24 May 2019 16:07:10	U	SMPL
K2997-03 - 1	DPC-81626-FB-03	105	0.0253	-	7470A	PPB	24 May 2019 16:09:17	U	SMPL
K2997-04 - 1	DPC-81626-FB-04	98	0.0237	-	7470A	PPB	24 May 2019 16:11:24	U	SMPL
K2997-05 - 1	DPC-81626-FB-05	100	0.0241	-	7470A	PPB	24 May 2019 16:13:32	U	SMPL
K3008-07 - 1	COMP-19	79	0.0192	-	7470A	PPB	24 May 2019 16:15:40	U	SMPL
K3008-08 - 1	COMP-20	92	0.0222	-	7470A	PPB	24 May 2019 16:17:47	U	SMPL
CCV02 - 1	CCV02	22165	5.2137	-	7470A	PPB	24 May 2019 16:19:53	U	SMPL
CCB02 - 1	CCB02	-48	-0.0107	-	7470A	PPB	24 May 2019 16:22:00	U	SMPL
K3008-09 - 1	COMP-21	114	0.0274	-	7470A	PPB	24 May 2019 16:24:07	U	SMPL
PB120062BL - 1	PBW	6	0.0020	-	7470A	PPB	24 May 2019 16:26:13	U	SMPL
PB120062BS - 1	LCSW	17748	4.1749	-	7470A	PPB	24 May 2019 16:28:20	U	SMPL
K2970-18 - 1	TP-10	111	0.0267	-	7470A	PPB	24 May 2019 16:30:27	U	SMPL
K2970-18DUP - 1	TP-10DUP	190	0.0453	-	7470A	PPB	24 May 2019 16:32:34	U	SMPL
K2970-18MS - 1	TP-10MS	19010	4.4717	-	7470A	PPB	24 May 2019 16:34:41	U	SMPL
K2970-18MSD - 1	TP-10MSD	19031	4.4766	-	7470A	PPB	24 May 2019 16:36:48	U	SMPL
K2994-18 - 1	TP-7	45	0.0112	-	7470A	PPB	24 May 2019 16:38:56	U	SMPL
PB120063BL - 1	PBW	79	0.0192	-	7470A	PPB	24 May 2019 16:41:05	U	SMPL
PB120063BS - 1	LCSW	17700	4.1636	-	7470A	PPB	24 May 2019 16:43:12	U	SMPL
CCV03 - 1	CCV03	21914	5.1547	-	7470A	PPB	24 May 2019 16:45:18	U	SMPL
CCB03 - 1	CCB03	-52	-0.0116	-	7470A	PPB	24 May 2019 16:47:25	U	SMPL
K2643-10 - 1	OR-03-052319-A	424	0.1003	-	7470A	PPB	24 May 2019 16:49:31	U	SMPL
K2643-10DUP - 1	OR-03-052319-ADUP	429	0.1015	-	7470A	PPB	24 May 2019 16:51:37	U	SMPL
K2643-10MS - 1	OR-03-052319-AMS	17634	4.1481	-	7470A	PPB	24 May 2019 16:53:44	U	SMPL
K2643-10MSD - 1	OR-03-052319-AMSD	17841	4.1967	-	7470A	PPB	24 May 2019 16:55:51	U	SMPL
K2643-12 - 1	OR-03-052319-B	33	0.0084	-	7470A	PPB	24 May 2019 16:57:59	U	SMPL
K3019-03 - 1	RT-3422	109	0.0262	-	7470A	PPB	24 May 2019 17:00:06	U	SMPL
K3019-06 - 1	RBR200036	98	0.0237	-	7470A	PPB	24 May 2019 17:02:14	U	SMPL
K3019-09 - 1	RT-1465	243	0.0578	-	7470A	PPB	24 May 2019 17:04:22	U	SMPL
K3023-01 - 1	SSSI-0523-S-TCLP-11	651	0.1537	-	7470A	PPB	24 May 2019 17:06:31	U	SMPL
K3026-04 - 1	TP-5-S	631	0.1490	-	7470A	PPB	24 May 2019 17:08:38	U	SMPL
CCV04 - 1	CCV04	22161	5.2128	-	7470A	PPB	24 May 2019 17:19:24	U	SMPL
CCB04 - 1	CCB04	-60	-0.0135	-	7470A	PPB	24 May 2019 17:21:31	U	SMPL
K3026-08 - 1	TP-5-D	221	0.0526	-	7470A	PPB	24 May 2019 17:23:38	U	SMPL
K3026-16 - 1	TP-3-S	167	0.0399	-	7470A	PPB	24 May 2019 17:25:47	U	SMPL
K3035-01 - 1	OIL-WATER-SEPERATOR(OWS)-3	79	0.0192	-	7470A	PPB	24 May 2019 17:28:02	U	SMPL
PB120061TB - 1	PB119981TB	108	0.0260	-	7470A	PPB	24 May 2019 17:30:08	U	SMPL
PB120062TB - 1	PB119983TB	112	0.0269	-	7470A	PPB	24 May 2019 17:32:16	U	SMPL
PB120063TB - 1	PB120020TB	43	0.0107	-	7470A	PPB	24 May 2019 17:34:23	U	SMPL
K2647-12LX5 - 1		45	0.0112	-	7470A	PPB	24 May 2019 17:36:31	U	SMPL
K2647-12A - 1		18033	4.2419	-	7470A	PPB	24 May 2019 17:38:40	U	SMPL
K2970-18LX5 - 1		-15	-0.0029	-	7470A	PPB	24 May 2019 17:40:52	U	SMPL
K2970-18A - 1		19100	4.4929	-	7470A	PPB	24 May 2019 17:43:00	U	SMPL
CCV05 - 1	CCV05	21789	5.1253	-	7470A	PPB	24 May 2019 17:48:38	U	SMPL
CCB05 - 1	CCB05	1	0.0008	-	7470A	PPB	24 May 2019 17:50:45	U	SMPL
K2643-10LX5 - 1		99	0.0239	-	7470A	PPB	24 May 2019 17:52:52	U	SMPL
K2643-10A - 1		17593	4.1384	-	7470A	PPB	24 May 2019 17:54:59	U	SMPL
CCV06 - 1	CCV06	21530	5.0644	-	7470A	PPB	24 May 2019 17:57:07	U	SMPL
CCB06 - 1	CCB06	-60	-0.0135	-	7470A	PPB	24 May 2019 17:59:14	U	SMPL