

21103058

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : As

Instrument ID : Konelab

5/29/2019 13:25

Test: Total CN

Ng/d

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.674	0.0	0.102	
ICB1	0.680	0.0	0.004	
CCV1	237.252	0.0	0.248	
CCB1	0.851	0.0	0.004	
PB120154BL	0.715	0.0	0.004	
PB120154BS	98.092	0.0	0.104	
LOWPB120154	10.532	0.0	0.014	
HIGHPB120154	484.667	0.0	0.503	
K2433-01	0.953	0.0	0.004	
K2433-01DUP	0.865	0.0	0.004	
K2433-01MS	32.791	0.0	0.037	
K2433-01MSD	32.946	0.0	0.037	
K3054-01	1.241	0.0	0.004	
K3074-05	1.395	0.0	0.005	
CCV2	238.676	0.0	0.249	
CCB2	0.979	0.0	0.004	
K3074-09	0.961	0.0	0.004	
K3075-01	0.892	0.0	0.004	
K3075-03	0.823	0.0	0.004	
K3075-05	0.745	0.0	0.004	
K3075-07	1.124	0.0	0.004	
K3075-09	0.836	0.0	0.004	
CCV3	254.236	0.0	0.265	
CCB3	0.711	0.0	0.004	

N	24
Mean	62.443
SD	121.6326
CV%	194.79

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/29/2019 11:26


Test Total CN

Accepted 5/29/2019 11:26

Factor 969.6
Bias 0.003

Coeff. of det. 0.999957

Errors

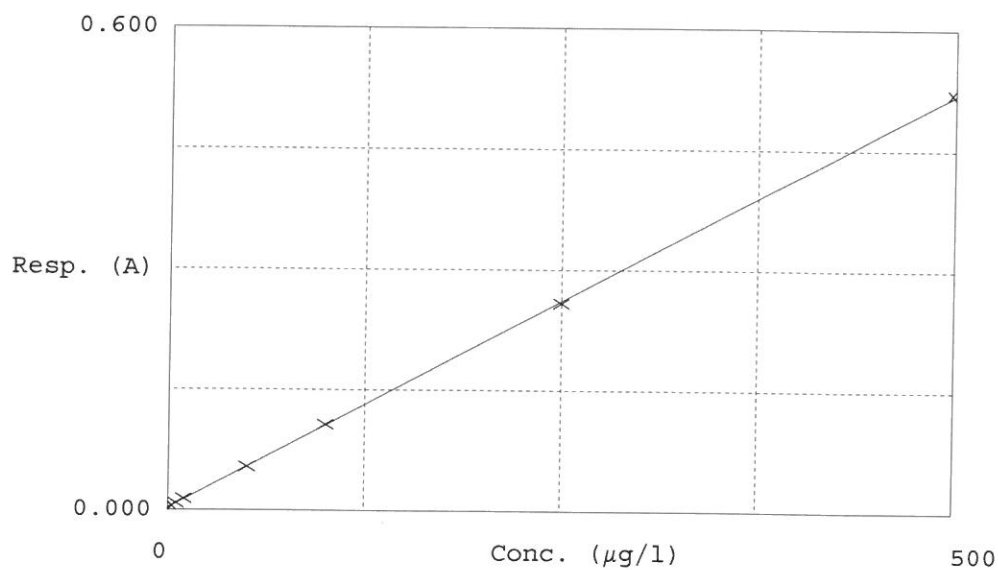

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.5157	0.0000	
2	5.0PPBCN	0.009	5.1871	5.0000	
3	10PPBCN	0.014	10.6668	10.0000	
4	50PPBCN	0.054	49.3869	50.0000	
5	100PPBCN	0.107	100.5367	100.0000	
6	250PPBCN	0.258	247.5362	250.0000	
7	500PPBCN	0.520	501.1706	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Wed May 29 13:13:11 2019

Wed May 29 13:24:39 2019

AS

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.5157	µg/l	5/29/2019 11:15:55	
5.0PPBCN	A	Total CN	P	5.1871	µg/l	5/29/2019 11:15:56	
10PPBCN	A	Total CN	P	10.6668	µg/l	5/29/2019 11:15:57	
50PPBCN	A	Total CN	P	49.3869	µg/l	5/29/2019 11:15:58	
100PPBCN	A	Total CN	P	100.5367	µg/l	5/29/2019 11:15:59	
250PPBCN	A	Total CN	P	247.5362	µg/l	5/29/2019 11:16:00	
500PPBCN	A	Total CN	P	501.1706	µg/l	5/29/2019 11:16:01	
ICV1	S	Total CN	P	95.6737	µg/l	5/29/2019 13:13:11	
ICB1	S	Total CN	P	0.6801	µg/l	5/29/2019 13:13:12	
CCV1	S	Total CN	P	237.2516	µg/l	5/29/2019 13:13:13	
CCB1	S	Total CN	P	0.8512	µg/l	5/29/2019 13:13:14	
PB120154BL	S	Total CN	P	0.7149	µg/l	5/29/2019 13:13:15	
PB120154BS	S	Total CN	P	98.0922	µg/l	5/29/2019 13:13:16	
LOWPB120154	S	Total CN	P	10.5323	µg/l	5/29/2019 13:13:17	
HIGHPB120154	S	Total CN	P	484.6666	µg/l	5/29/2019 13:13:18	
K2433-01	S	Total CN	P	0.9526	µg/l	5/29/2019 13:13:19	
K2433-01DUP	S	Total CN	P	0.8647	µg/l	5/29/2019 13:13:20	
K2433-01MS	S	Total CN	P	32.7914	µg/l	5/29/2019 13:13:21	
K2433-01MSD	S	Total CN	P	32.9464	µg/l	5/29/2019 13:20:46	
K3054-01	S	Total CN	P	1.2414	µg/l	5/29/2019 13:20:47	
K3074-05	S	Total CN	P	1.3948	µg/l	5/29/2019 13:20:48	
CCV2	S	Total CN	P	238.6764	µg/l	5/29/2019 13:20:49	
CCB2	S	Total CN	P	0.9785	µg/l	5/29/2019 13:20:50	
K3074-09	S	Total CN	P	0.9613	µg/l	5/29/2019 13:20:51	
K3075-01	S	Total CN	P	0.8915	µg/l	5/29/2019 13:20:52	
K3075-03	S	Total CN	P	0.8234	µg/l	5/29/2019 13:20:53	
K3075-05	S	Total CN	P	0.7447	µg/l	5/29/2019 13:20:54	
K3075-07	S	Total CN	P	1.1239	µg/l	5/29/2019 13:20:55	
K3075-09	S	Total CN	P	0.836	µg/l	5/29/2019 13:20:56	
CCV3	S	Total CN	P	254.2361	µg/l	5/29/2019 13:24:37	
CCB3	S	Total CN	P	0.7112	µg/l	5/29/2019 13:24:38	