

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/29/2019 14:06

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.167	0.0	0.102	
ICB1	0.881	0.0	0.004	
CCV1	238.077	0.0	0.249	
CCB1	0.721	0.0	0.004	
PB120155BL	0.827	0.0	0.004	
PB120155BS	97.570	0.0	0.104	
MIDPB120155	240.662	0.0	0.251	
K3070-07	10.033	0.0	0.014	
K3070-07DUP	9.907	0.0	0.013	
K3070-07MS	37.452	0.0	0.042	
K3070-07MSD	38.096	0.0	0.042	
CCV3	254.355	0.0	0.266	
CCB3	0.653	0.0	0.004	

N	13
Mean	78.877
SD	100.0992
CV%	126.91

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/29/2019 14:11


Test Total CN

Accepted 5/29/2019 11:26

Factor 969.6
Bias 0.003

Coeff. of det. 0.999957

Errors

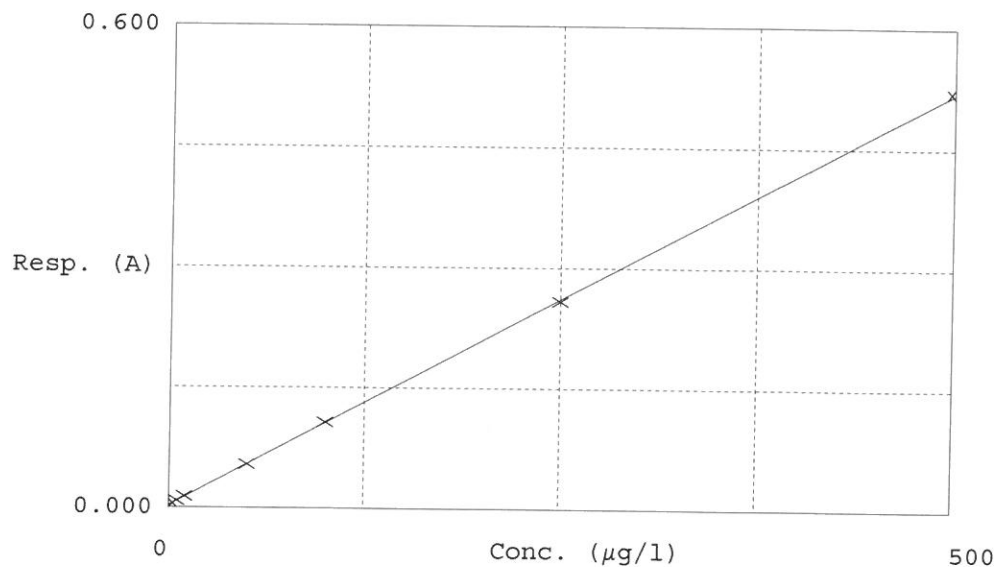

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.5157	0.0000	
2	5.0PPBCN	0.009	5.1871	5.0000	
3	10PPBCN	0.014	10.6668	10.0000	
4	50PPBCN	0.054	49.3869	50.0000	
5	100PPBCN	0.107	100.5367	100.0000	
6	250PPBCN	0.258	247.5362	250.0000	
7	500PPBCN	0.520	501.1706	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Wed May 29 13:56:21 2019

Wed May 29 14:00:43 2019

✓AS

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.5157	µg/l	5/29/2019 11:15:55	
5.0PPBCN	A	Total CN	P	5.1871	µg/l	5/29/2019 11:15:56	
10PPBCN	A	Total CN	P	10.6668	µg/l	5/29/2019 11:15:57	
50PPBCN	A	Total CN	P	49.3869	µg/l	5/29/2019 11:15:58	
100PPBCN	A	Total CN	P	100.5367	µg/l	5/29/2019 11:15:59	
250PPBCN	A	Total CN	P	247.5362	µg/l	5/29/2019 11:16:0	
500PPBCN	A	Total CN	P	501.1706	µg/l	5/29/2019 11:16:1	
ICV1	S	Total CN	P	96.1669	µg/l	5/29/2019 13:56:21	
ICB1	S	Total CN	P	0.8813	µg/l	5/29/2019 13:56:22	
CCV1	S	Total CN	P	238.0775	µg/l	5/29/2019 13:56:23	
CCB1	S	Total CN	P	0.721	µg/l	5/29/2019 13:56:24	
PB120155BL	S	Total CN	P	0.8266	µg/l	5/29/2019 13:56:25	
PB120155BS	S	Total CN	P	97.5702	µg/l	5/29/2019 13:56:26	
MIDPB120155	S	Total CN	P	240.662	µg/l	5/29/2019 13:56:27	
K3070-07	S	Total CN	P	10.0327	µg/l	5/29/2019 13:56:28	
K3070-07DUP	S	Total CN	P	9.9066	µg/l	5/29/2019 13:56:29	
K3070-07MS	S	Total CN	P	37.4523	µg/l	5/29/2019 14:00:40	
K3070-07MSD	S	Total CN	P	38.0961	µg/l	5/29/2019 14:00:41	
CCV3	S	Total CN	P	254.3551	µg/l	5/29/2019 14:00:42	
CCB3	S	Total CN	P	0.6533	µg/l	5/29/2019 14:00:43	