

13103067

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/29/2019 15:06

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.884	0.0	0.101	
ICB1	0.822	0.0	0.004	
CCV1	235.629	0.0	0.246	
CCB1	0.608	0.0	0.004	
PB120166BL	0.962	0.0	0.004	
PB120166BS	96.453	0.0	0.103	
K3072-01	0.809	0.0	0.004	
K3072-01DUP	0.596	0.0	0.004	
K3072-01MS	29.465	0.0	0.034	
K3072-01MSD	29.277	0.0	0.033	
K3072-03	1.212	0.0	0.004	
K3072-02	1.005	0.0	0.004	
K3072-04	1.027	0.0	0.004	
K3072-05	1.143	0.0	0.004	
CCV2	238.653	0.0	0.249	
CCB2	0.781	0.0	0.004	
K3072-06	1.177	0.0	0.004	
K3072-07	0.763	0.0	0.004	
K3072-08	1.027	0.0	0.004	
CCV3	236.726	0.0	0.247	
CCB3	0.454	0.0	0.004	

N 21
Mean 46.356
SD 84.6854
CV% 182.69

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

5/29/2019 15:09


Test Total CN

Accepted 5/29/2019 11:26

Factor 969.6
Bias 0.003

Coeff. of det. 0.999957

Errors

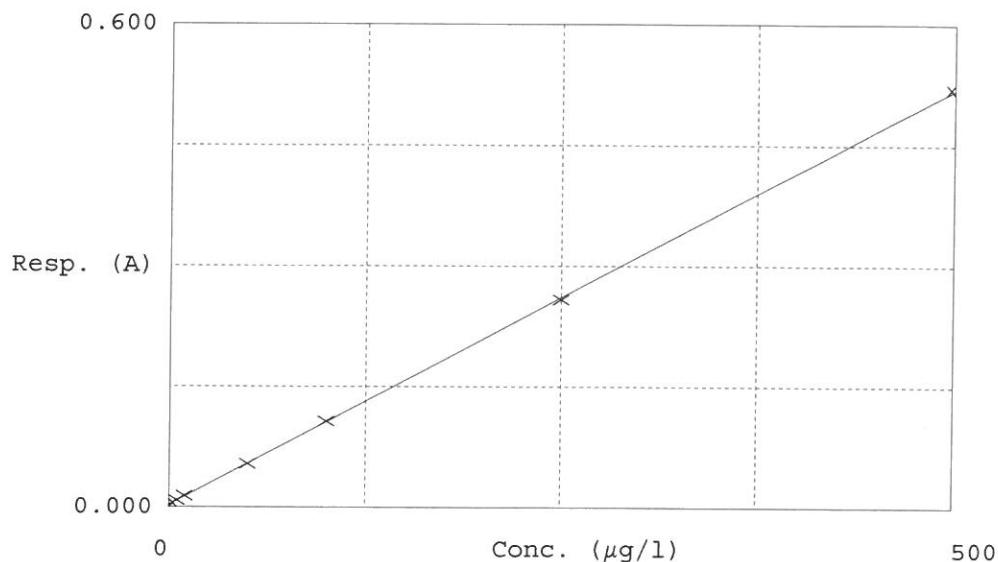

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.5157	0.0000	
2	5.0PPBCN	0.009	5.1871	5.0000	
3	10PPBCN	0.014	10.6668	10.0000	
4	50PPBCN	0.054	49.3869	50.0000	
5	100PPBCN	0.107	100.5367	100.0000	
6	250PPBCN	0.258	247.5362	250.0000	
7	500PPBCN	0.520	501.1706	500.0000	

AS

Aquakem v. 7.2AQ1

Results from time period:

Wed May 29 14:50:08 2019

Wed May 29 15:01:07 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.5157	µg/l	5/29/2019 11:15:55	
5.0PPBCN	A	Total CN	P	5.1871	µg/l	5/29/2019 11:15:56	
10PPBCN	A	Total CN	P	10.6668	µg/l	5/29/2019 11:15:57	
50PPBCN	A	Total CN	P	49.3869	µg/l	5/29/2019 11:15:58	
100PPBCN	A	Total CN	P	100.5367	µg/l	5/29/2019 11:15:59	
250PPBCN	A	Total CN	P	247.5362	µg/l	5/29/2019 11:16:00	
500PPBCN	A	Total CN	P	501.1706	µg/l	5/29/2019 11:16:01	
ICV1	S	Total CN	P	94.8845	µg/l	5/29/2019 14:50:08	
ICB1	S	Total CN	P	0.8219	µg/l	5/29/2019 14:50:09	
CCV1	S	Total CN	P	235.6288	µg/l	5/29/2019 14:50:10	
CCB1	S	Total CN	P	0.608	µg/l	5/29/2019 14:50:11	
PB120166BL	S	Total CN	P	0.9615	µg/l	5/29/2019 14:50:12	
PB120166BS	S	Total CN	P	96.4531	µg/l	5/29/2019 14:50:13	
K3072-01	S	Total CN	P	0.8087	µg/l	5/29/2019 14:50:14	
K3072-01DUP	S	Total CN	P	0.5958	µg/l	5/29/2019 14:50:15	
K3072-01MS	S	Total CN	P	29.4653	µg/l	5/29/2019 14:50:16	
K3072-01MSD	S	Total CN	P	29.2771	µg/l	5/29/2019 14:50:17	
K3072-03	S	Total CN	P	1.2123	µg/l	5/29/2019 14:50:18	
K3072-02	S	Total CN	P	1.0053	µg/l	5/29/2019 14:57:43	
K3072-04	S	Total CN	P	1.0271	µg/l	5/29/2019 14:57:44	
K3072-05	S	Total CN	P	1.1434	µg/l	5/29/2019 14:57:45	
CCV2	S	Total CN	P	238.6527	µg/l	5/29/2019 14:57:46	
CCB2	S	Total CN	P	0.7813	µg/l	5/29/2019 14:57:47	
K3072-06	S	Total CN	P	1.177	µg/l	5/29/2019 14:57:48	
K3072-07	S	Total CN	P	0.7632	µg/l	5/29/2019 14:57:49	
K3072-08	S	Total CN	P	1.027	µg/l	5/29/2019 14:57:50	
CCV3	S	Total CN	P	236.7262	µg/l	5/29/2019 14:57:53	
CCB3	S	Total CN	P	0.4542	µg/l	5/29/2019 15:01:06	