

dB103227

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/6/2019 10:50

Test: Phenolics-

mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.989	0.0	0.127	
ICB1	-0.006	0.0	0.020	
CCV1	0.955	0.0	0.123	
CCB1	-0.008	0.0	0.019	
PB120366BL	-0.009	0.0	0.019	
PB120366BS	0.995	0.0	0.127	
K3182-07	-0.006	0.0	0.020	
K3182-07DUP	-0.006	0.0	0.020	
K3182-07MS	0.875	0.0	0.115	
K3182-07MSD	0.875	0.0	0.115	
K3191-01	-0.012	0.0	0.019	
CCV2	0.966	0.0	0.124	
CCB2	-0.007	0.0	0.020	

N	13
Mean	0.431
SD	0.4943
CV%	114.70

AS

Aquakem v. 7.2AQ1

Results from time period:

Thu Jun 06 09:02:48 2019

Thu Jun 06 10:40:38 2019

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0507	mg/l	6/6/2019 9:02:48	
0.1PPM	A	Phenolics-	P	0.1028	mg/l	6/6/2019 9:02:49	
0.25PPM	A	Phenolics-	P	0.2482	mg/l	6/6/2019 9:02:50	
0.50PPM	A	Phenolics-	P	0.4991	mg/l	6/6/2019 9:02:51	
1.0PPM	A	Phenolics-	P	0.9978	mg/l	6/6/2019 9:02:52	
2.0PPM	A	Phenolics-	P	2.0014	mg/l	6/6/2019 9:02:53	
ICV1	S	Phenolics-	P	0.9894	mg/l	6/6/2019 10:35:41	
ICB1	S	Phenolics-	P	-0.0056	mg/l	6/6/2019 10:35:42	
CCV1	S	Phenolics-	P	0.9554	mg/l	6/6/2019 10:35:43	
CCB1	S	Phenolics-	P	-0.008	mg/l	6/6/2019 10:35:44	
PB120366BL	S	Phenolics-	P	-0.0092	mg/l	6/6/2019 10:35:45	
PB120366BS	S	Phenolics-	P	0.9953	mg/l	6/6/2019 10:35:46	
K3182-07	S	Phenolics-	P	-0.0059	mg/l	6/6/2019 10:35:47	
K3182-07DUP	S	Phenolics-	P	-0.0061	mg/l	6/6/2019 10:35:48	
K3182-07MS	S	Phenolics-	P	0.8752	mg/l	6/6/2019 10:35:49	
K3182-07MSD	S	Phenolics-	P	0.8749	mg/l	6/6/2019 10:35:50	
K3191-01	S	Phenolics-	P	-0.0119	mg/l	6/6/2019 10:35:51	
CCV2	S	Phenolics-	P	0.9656	mg/l	6/6/2019 10:40:36	
CCB2	S	Phenolics-	P	-0.0066	mg/l	6/6/2019 10:40:37	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/6/2019 9:47


Test Phenolics-

Accepted 6/6/2019 9:47

Factor 9.281
Bias 0.020

Coeff. of det. 0.999993

Errors

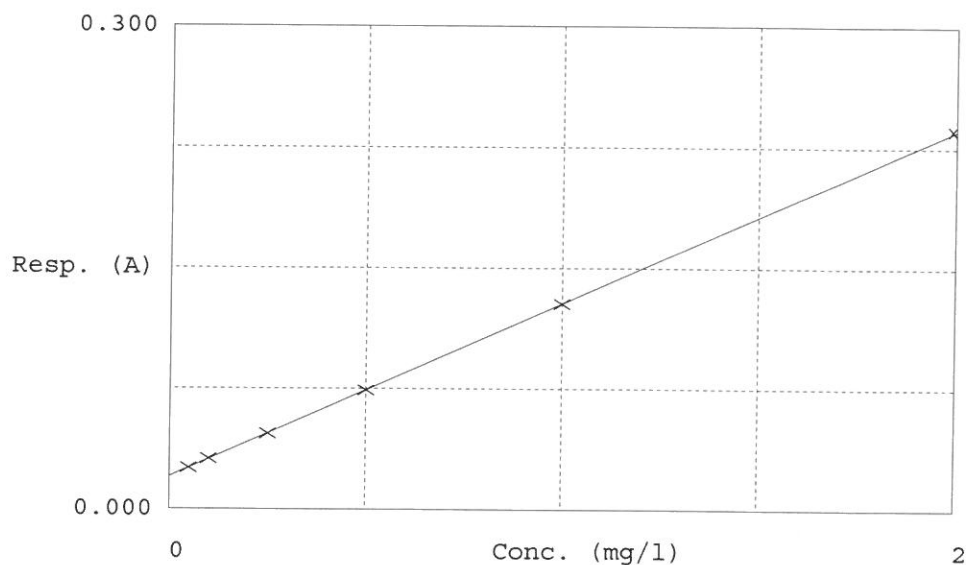

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.026	0.0507	0.0500	
2	Phenol-2	0.031	0.1028	0.1000	
3	Phenol-2	0.047	0.2482	0.2500	
4	Phenol-2	0.074	0.4991	0.5000	
5	Phenol-2	0.128	0.9978	1.0000	
6	Phenol-2	0.236	2.0014	2.0000	