

LB103239


7471B

INSTRUMENT ID : CU1

Linear

 μ Abs. :

62986

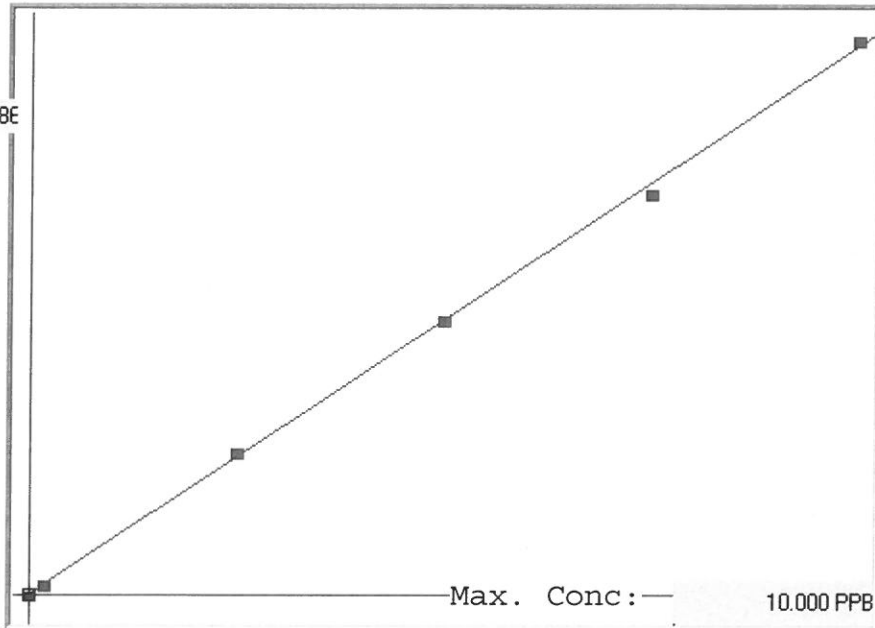

A= 0.0000e+000

B= 1.6050e-004

C= -1.1317e-002

Rho= 0.9996820

Accept = Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.008	-0.008	19	0.000	19				
0.2	0.200	0.178	-0.022	1181	0.0 %	1181				
2.5	2.500	2.595	0.095	16238	0.0 %	16238				
5.0	5.000	5.017	0.017	31331	0.0 %	31331				
7.5	7.500	7.320	-0.180	45676	0.0 %	45676				
10.0	10.000	10.098	0.098	62986	0.0 %	62986				

LB103239 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 06 Jun 2019 14:05:12

Sample ID	Extended ID	µ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	S0-0	19	-	0.00007471B	PPB	06 Jun 2019 14:08:28	S	Std
0.2 - 1	S0-2	1181	-	0.20007471B	PPB	06 Jun 2019 14:10:46	S	Std
2.5 - 1	S2-5	16238	-	2.50007471B	PPB	06 Jun 2019 14:13:05	S	Std
5.0 - 1	S5-0	31331	-	5.00007471B	PPB	06 Jun 2019 14:15:22	S	Std
7.5 - 1	S7-5	45676	-	7.50007471B	PPB	06 Jun 2019 14:17:39	S	Std
10.0 - 1	S10-0	62986	-	10.00007471B	PPB	06 Jun 2019 14:24:20	S	Std
ICV77 - 1	ICV77	25904	4.1463	-7471B	PPB	06 Jun 2019 14:28:52	U	SMPL
ICB77 - 1	ICB77	-80	-0.0242	-7471B	PPB	06 Jun 2019 14:31:08	U	SMPL
CCV89 - 1	CCV89	32119	5.1438	-7471B	PPB	06 Jun 2019 14:33:23	U	SMPL
CCB89 - 1	CCB89	-96	-0.0267	-7471B	PPB	06 Jun 2019 14:35:39	U	SMPL
CRA - 1	CRA	1174	0.1771	-7471B	PPB	06 Jun 2019 14:37:55	U	SMPL
HighStd - 1	HighStd	63597	10.1961	-7471B	PPB	06 Jun 2019 14:40:11	U	SMPL
ChkStd - 1	ChkStd	43169	6.9174	-7471B	PPB	06 Jun 2019 14:42:27	U	SMPL
PB120386BL - 1	PBS	-180	-0.0402	-7471B	PPB	06 Jun 2019 14:44:44	U	SMPL
PB120386BS - 1	LCSS	24142	3.8635	-7471B	PPB	06 Jun 2019 14:47:02	U	SMPL
K3153-01 - 1	HR-05-060519-A	5770	0.9148	-7471B	PPB	06 Jun 2019 14:49:19	U	SMPL
K3153-01DUP - 1	HR-05-060519-ADUP	5836	0.9254	-7471B	PPB	06 Jun 2019 14:51:36	U	SMPL
K3153-01MS - 1	HR-05-060519-AMS	31625	5.0645	-7471B	PPB	06 Jun 2019 14:53:53	U	SMPL
K3153-01MSD - 1	HR-05-060519-AMSD	30370	4.8631	-7471B	PPB	06 Jun 2019 14:56:11	U	SMPL
K3153-03 - 1	HR-05-060519-B	2986	0.4679	-7471B	PPB	06 Jun 2019 14:58:27	U	SMPL
CCV90 - 1	CCV90	32063	5.1348	-7471B	PPB	06 Jun 2019 15:00:44	U	SMPL
CCB90 - 1	CCB90	-70	-0.0226	-7471B	PPB	06 Jun 2019 15:03:00	U	SMPL
K3153-05 - 1	HR-05-060519-C	4831	0.7641	-7471B	PPB	06 Jun 2019 15:05:16	U	SMPL
K3156-01 - 1	HD-02-060519	1311	0.1991	-7471B	PPB	06 Jun 2019 15:07:32	U	SMPL
K3192-01 - 1	CULVER-CBTC-WC1B-060419	6950	1.1042	-7471B	PPB	06 Jun 2019 15:09:48	U	SMPL
K3211-01 - 1	RBR-20002	1153	0.1737	-7471B	PPB	06 Jun 2019 15:12:04	U	SMPL
K3211-03 - 1	RBR-200050	3087	0.4842	-7471B	PPB	06 Jun 2019 15:14:21	U	SMPL
K3211-05 - 1	RT-5124	2493	0.3888	-7471B	PPB	06 Jun 2019 15:16:37	U	SMPL
K3211-07 - 1	RBR-200052	2115	0.3281	-7471B	PPB	06 Jun 2019 15:18:54	U	SMPL
K3216-01 - 1	CONCRETE-COMP-1	149	0.0126	-7471B	PPB	06 Jun 2019 15:21:12	U	SMPL
K3216-03 - 1	CONCRETE-COMP-2	157	0.0139	-7471B	PPB	06 Jun 2019 15:23:30	U	SMPL
K3218-01 - 1	RBR-200035	837	0.1230	-7471B	PPB	06 Jun 2019 15:25:46	U	SMPL
CCV91 - 1	CCV91	31957	5.1178	-7471B	PPB	06 Jun 2019 15:28:02	U	SMPL
CCB91 - 1	CCB91	-53	-0.0198	-7471B	PPB	06 Jun 2019 15:30:17	U	SMPL
K3218-04 - 1	RBR-200027	1858	0.2869	-7471B	PPB	06 Jun 2019 15:32:33	U	SMPL
K3218-07 - 1	RT-1873	2414	0.3761	-7471B	PPB	06 Jun 2019 15:34:49	U	SMPL
K3153-01LX5 - 1		1117	0.1680	-7471B	PPB	06 Jun 2019 15:37:05	U	SMPL
K3153-01A - 1		31166	4.9909	-7471B	PPB	06 Jun 2019 15:39:21	U	SMPL
CCV92 - 1	CCV92	31400	5.0284	-7471B	PPB	06 Jun 2019 15:41:37	U	SMPL
CCB92 - 1	CCB92	-84	-0.0248	-7471B	PPB	06 Jun 2019 15:43:54	U	SMPL