

2103345

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/12/2019 8:59

Test: Total CN

Mg/d

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.376	0.0	0.100	
ICB1	0.427	0.0	0.004	
CCV1	241.208	0.0	0.245	
CCB1	0.308	0.0	0.004	
PB120479BL	0.361	0.0	0.004	
PB120479BS	96.805	0.0	0.100	
HIGHPB120479	489.885	0.0	0.493	
K3163-05	0.925	0.0	0.004	
K3163-05DUP	0.781	0.0	0.004	
K3163-05MS	25.009	0.0	0.028	
K3163-05MSD	25.534	0.0	0.029	
K3163-07	1.348	0.0	0.005	
K3271-02	1.126	0.0	0.004	
CCV2	243.885	0.0	0.247	
CCB2	0.601	0.0	0.004	
K3282-01	0.503	0.0	0.004	
K3283-01	1.075	0.0	0.004	
LOWPB120479	10.156	0.0	0.014	
CCV3	257.535	0.0	0.261	
CCB3	0.697	0.0	0.004	

N 20
Mean 74.727
SD 132.2552
CV% 176.98

AS

Aquakem v. 7.2AQ1

Results from time period:

Wed Jun 12 07:24:56 2019

Wed Jun 12 08:55:31 2019

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.1829	µg/l	6/12/2019 7:55:02	
5.0PPBCN	A	Total CN	P	5.1079	µg/l	6/12/2019 7:55:03	
10PPBCN	A	Total CN	P	9.8613	µg/l	6/12/2019 7:55:04	
50PPBCN	A	Total CN	P	50.3495	µg/l	6/12/2019 7:55:05	
100PPBCN	A	Total CN	P	100.1529	µg/l	6/12/2019 7:55:06	
250PPBCN	A	Total CN	P	249.5503	µg/l	6/12/2019 7:55:07	
500PPBCN	A	Total CN	P	500.161	µg/l	6/12/2019 7:55:08	
ICV1	S	Total CN	P	96.376	µg/l	6/12/2019 8:29:07	
ICB1	S	Total CN	P	0.4274	µg/l	6/12/2019 8:29:08	
CCV1	S	Total CN	P	241.2077	µg/l	6/12/2019 8:29:09	
CCB1	S	Total CN	P	0.3083	µg/l	6/12/2019 8:29:10	
PB120479BL	S	Total CN	P	0.3611	µg/l	6/12/2019 8:29:11	
PB120479BS	S	Total CN	P	96.8054	µg/l	6/12/2019 8:29:12	
HIGHPB120479	S	Total CN	P	489.8854	µg/l	6/12/2019 8:29:14	
K3163-05	S	Total CN	P	0.9251	µg/l	6/12/2019 8:29:15	
K3163-05DUP	S	Total CN	P	0.7814	µg/l	6/12/2019 8:29:16	
K3163-05MS	S	Total CN	P	25.0087	µg/l	6/12/2019 8:29:17	
K3163-05MSD	S	Total CN	P	25.5344	µg/l	6/12/2019 8:36:42	
K3163-07	S	Total CN	P	1.3479	µg/l	6/12/2019 8:36:43	
K3271-02	S	Total CN	P	1.1261	µg/l	6/12/2019 8:36:44	
CCV2	S	Total CN	P	243.8852	µg/l	6/12/2019 8:36:45	
CCB2	S	Total CN	P	0.6005	µg/l	6/12/2019 8:36:46	
K3282-01	S	Total CN	P	0.5026	µg/l	6/12/2019 8:36:47	
K3283-01	S	Total CN	P	1.0754	µg/l	6/12/2019 8:36:48	
LOWPB120479	S	Total CN	P	10.1558	µg/l	6/12/2019 8:55:29	
CCV3	S	Total CN	P	257.5355	µg/l	6/12/2019 8:55:30	
CCB3	S	Total CN	P	0.6969	µg/l	6/12/2019 8:55:31	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/12/2019 8:03


Test Total CN

Accepted 6/12/2019 8:03

Factor 1000
Bias 0.003

Coeff. of det. 0.999998

Errors

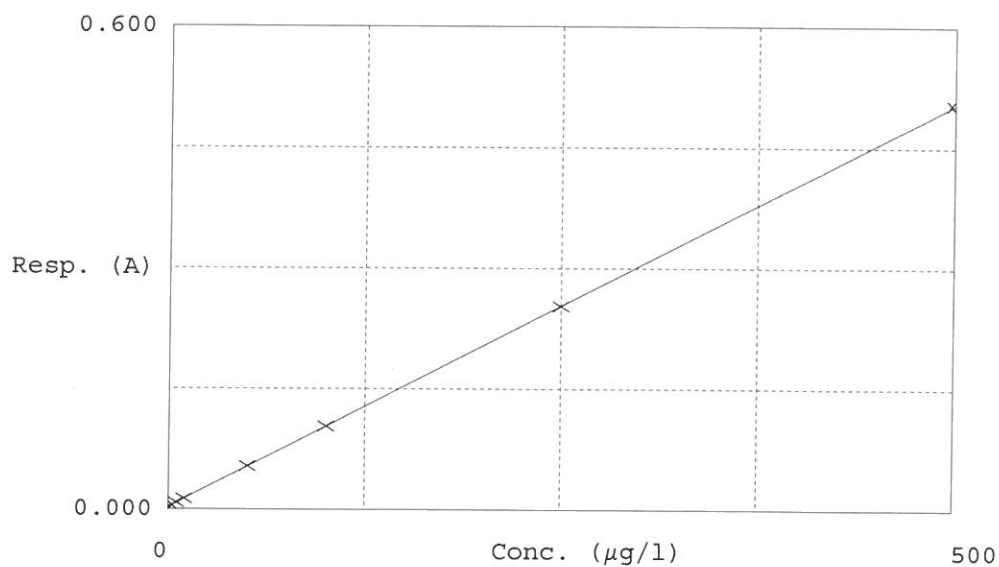

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.1829	0.0000	
2	5.0PPBCN	0.008	5.1079	5.0000	
3	10PPBCN	0.013	9.8613	10.0000	
4	50PPBCN	0.054	50.3495	50.0000	
5	100PPBCN	0.104	100.1529	100.0000	
6	250PPBCN	0.253	249.5503	250.0000	
7	500PPBCN	0.503	500.1610	500.0000	