

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/12/2019 12:47

Test: *Reactance*
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.945	0.0	0.100	
ICB1	0.489	0.0	0.004	
CCV1	242.531	0.0	0.246	
CCB1	0.338	0.0	0.004	
PB120510BL	0.476	0.0	0.004	
K3282-02	0.441	0.0	0.004	
K3282-02DUP	0.177	0.0	0.004	
K3283-03	0.339	0.0	0.004	
PB120545BL	0.284	0.0	0.004	
K3159-02	0.468	0.0	0.004	
K3159-02DUP	-0.406	0.0	0.003	
K3159-04	0.218	0.0	0.004	
K3285-03	0.297	0.0	0.004	
CCV2	258.437	0.0	0.262	
CCB2	0.323	0.0	0.004	

N 15
Mean 40.091
SD 89.0033
CV% 222.01

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/12/2019 13:01


Test Total CN

Accepted 6/12/2019 8:03

Factor 1000
Bias 0.003

Coeff. of det. 0.999998

Errors

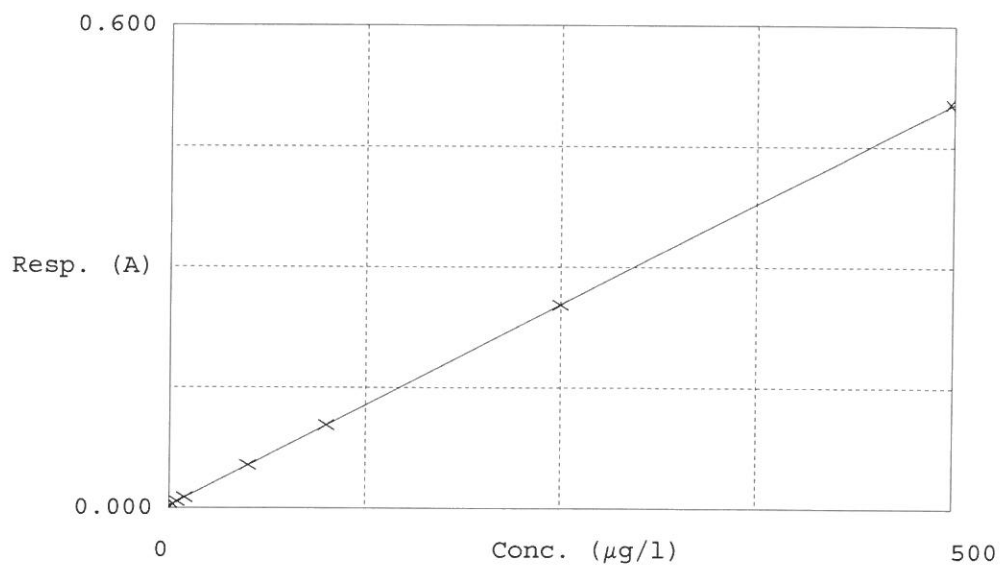

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.1829	0.0000	
2	5.0PPBCN	0.008	5.1079	5.0000	
3	10PPBCN	0.013	9.8613	10.0000	
4	50PPBCN	0.054	50.3495	50.0000	
5	100PPBCN	0.104	100.1529	100.0000	
6	250PPBCN	0.253	249.5503	250.0000	
7	500PPBCN	0.503	500.1610	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Wed Jun 12 12:41:41 2019

Wed Jun 12 12:46:03 2019

A3

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.1829	µg/l	6/12/2019 7:55:02	
5.OPPBCN	A	Reactive CN	P	5.1079	µg/l	6/12/2019 7:55:03	
10PPBCN	A	Reactive CN	P	9.8613	µg/l	6/12/2019 7:55:04	
50PPBCN	A	Reactive CN	P	50.3495	µg/l	6/12/2019 7:55:05	
100PPBCN	A	Reactive CN	P	100.1529	µg/l	6/12/2019 7:55:06	
250PPBCN	A	Reactive CN	P	249.5503	µg/l	6/12/2019 7:55:07	
500PPBCN	A	Reactive CN	P	500.161	µg/l	6/12/2019 7:55:08	
ICV1	S	Reactive CN	P	96.9453	µg/l	6/12/2019 12:41:41	
ICB1	S	Reactive CN	P	0.4889	µg/l	6/12/2019 12:41:42	
CCV1	S	Reactive CN	P	242.5309	µg/l	6/12/2019 12:41:43	
CCB1	S	Reactive CN	P	0.3385	µg/l	6/12/2019 12:41:44	
PB120510BL	S	Reactive CN	P	0.4758	µg/l	6/12/2019 12:41:45	
K3282-02	S	Reactive CN	P	0.4414	µg/l	6/12/2019 12:41:46	
K3282-02DUP	S	Reactive CN	P	0.1775	µg/l	6/12/2019 12:41:47	
K3283-03	S	Reactive CN	P	0.3388	µg/l	6/12/2019 12:41:48	
PB120545BL	S	Reactive CN	P	0.2839	µg/l	6/12/2019 12:41:49	
K3159-02	S	Reactive CN	P	0.4684	µg/l	6/12/2019 12:41:50	
K3159-02DUP	S	Reactive CN	P	-0.4058	µg/l	6/12/2019 12:41:51	
K3159-04	S	Reactive CN	P	0.2182	µg/l	6/12/2019 12:46:00	
K3285-03	S	Reactive CN	P	0.2969	µg/l	6/12/2019 12:46:01	
CCV2	S	Reactive CN	P	258.4372	µg/l	6/12/2019 12:46:02	
CCB2	S	Reactive CN	P	0.323	µg/l	6/12/2019 12:46:03	