

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/12/2019 15:46

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.958	0.0	0.125	
ICB1	0.002	0.0	0.020	
CCV1	0.981	0.0	0.128	
CCB1	0.001	0.0	0.020	
PB120493BL	-0.001	0.0	0.020	
PB120493BS	0.959	0.0	0.125	
K3265-13	0.006	0.0	0.021	
K3265-13DUP	0.005	0.0	0.021	
K3265-13MS	0.950	0.0	0.124	
K3265-13MSD	0.952	0.0	0.125	
CCV2	0.973	0.0	0.127	
CCB2	0.000	0.0	0.020	

N 12
Mean 0.482
SD 0.5012
CV% 103.94

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AB

Instrument ID : Konelab

6/12/2019 14:52


Test Phenolics-

Accepted 6/12/2019 14:52

Factor 9.114
Bias 0.020

Coeff. of det. 0.999803

Errors

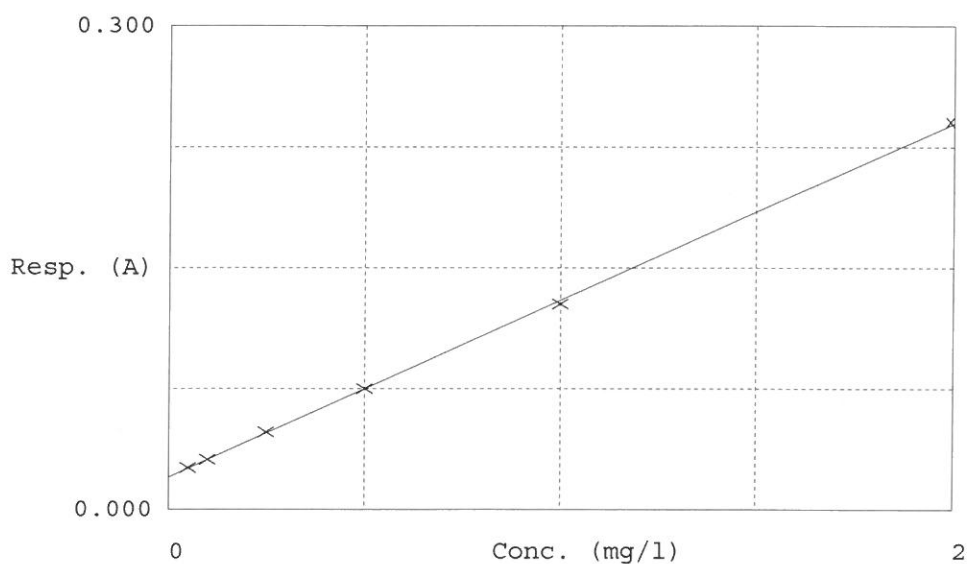

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.026	0.0544	0.0500	
2	Phenol-2	0.031	0.1004	0.1000	
3	Phenol-2	0.048	0.2557	0.2500	
4	Phenol-2	0.075	0.5007	0.5000	
5	Phenol-2	0.128	0.9797	1.0000	
6	Phenol-2	0.241	2.0091	2.0000	

Aquakem v. 7.2AQ1

Results from time period:

Wed Jun 12 14:32:30 2019

Wed Jun 12 15:25:04 2019

✓ A 3

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0544	mg/l	6/12/2019 14:51:17	
0.1PPM	A	Phenolics-	P	0.1004	mg/l	6/12/2019 14:51:18	
0.25PPM	A	Phenolics-	P	0.2557	mg/l	6/12/2019 14:51:19	
0.50PPM	A	Phenolics-	P	0.5007	mg/l	6/12/2019 14:51:20	
1.0PPM	A	Phenolics-	P	0.9797	mg/l	6/12/2019 14:51:21	
2.0PPM	A	Phenolics-	P	2.0091	mg/l	6/12/2019 14:51:22	
ICV1	S	Phenolics-	P	0.9578	mg/l	6/12/2019 15:20:07	
ICB1	S	Phenolics-	P	0.0025	mg/l	6/12/2019 15:20:08	
CCV1	S	Phenolics-	P	0.9813	mg/l	6/12/2019 15:20:09	
CCB1	S	Phenolics-	P	0.0014	mg/l	6/12/2019 15:20:10	
PB120493BL	S	Phenolics-	P	-0.0007	mg/l	6/12/2019 15:20:11	
PB120493BS	S	Phenolics-	P	0.959	mg/l	6/12/2019 15:20:12	
K3265-13	S	Phenolics-	P	0.0058	mg/l	6/12/2019 15:20:13	
K3265-13DUP	S	Phenolics-	P	0.0052	mg/l	6/12/2019 15:20:14	
K3265-13MS	S	Phenolics-	P	0.9497	mg/l	6/12/2019 15:20:17	
K3265-13MSD	S	Phenolics-	P	0.952	mg/l	6/12/2019 15:20:18	
CCV2	S	Phenolics-	P	0.9727	mg/l	6/12/2019 15:25:01	
CCB2	S	Phenolics-	P	0.0004	mg/l	6/12/2019 15:25:02	